




Pile Dynamics, Inc.

Transducer C127

Strain ($\mu\epsilon$)

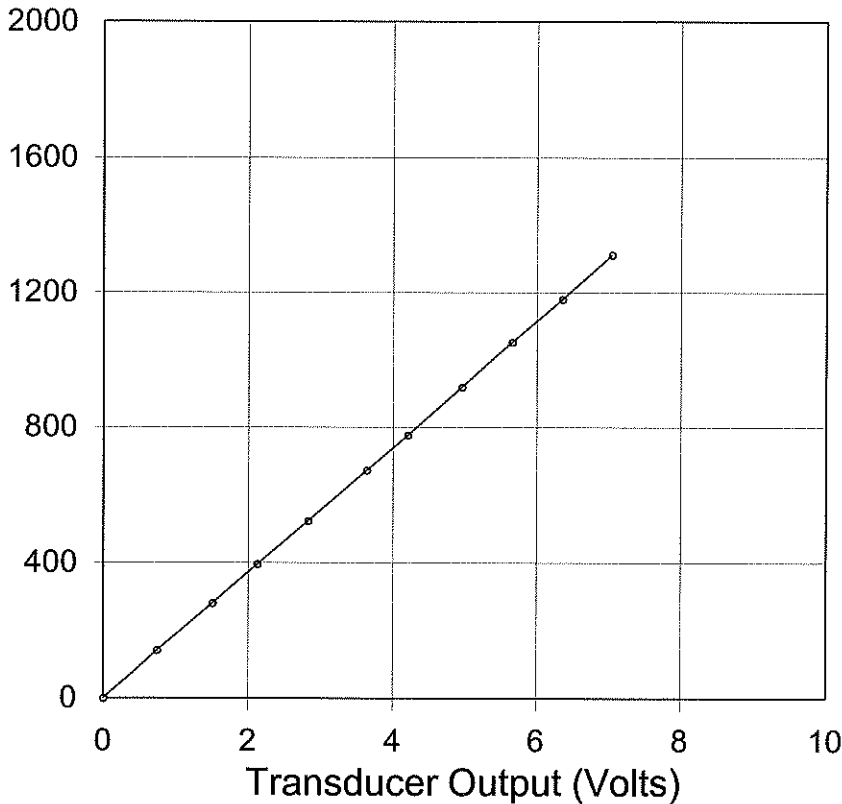

PDA Cal Factor (5.0 V)

92.9 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
142	0.73
280	1.50
394	2.12
523	2.82
672	3.63
777	4.20
919	4.95
1052	5.65
1180	6.35
1313	7.04

Shunt (60.4 K Ω)

2.5 V

General Factor

322.6 $\mu\epsilon/mV/V$

Calibrated by:

Handwritten signature

Calibrated on:

27-Feb-2008

Traceable to N.I.S.T.