




Pile Dynamics, Inc.

Transducer C129

Strain ($\mu\epsilon$)

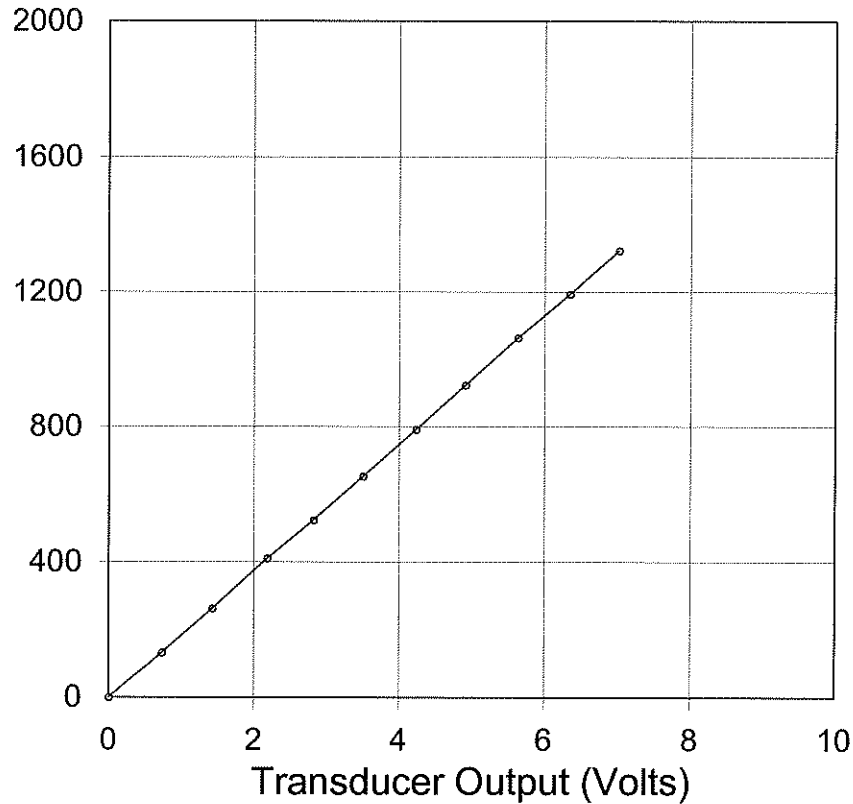

PDA Cal Factor (5.0 V)

94.4 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
134	0.72
264	1.42
409	2.18
522	2.81
652	3.50
791	4.23
922	4.91
1063	5.63
1193	6.34
1325	7.01

Shunt (60.4 K Ω)

2.5 V

General Factor

327.8 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2009 Version 1.3

Calibrated by:

Calibrated on:

21-Jun-2010