




Pile Dynamics, Inc.

Pile Dynamics, Inc. Transducer C132

Strain ($\mu\epsilon$)

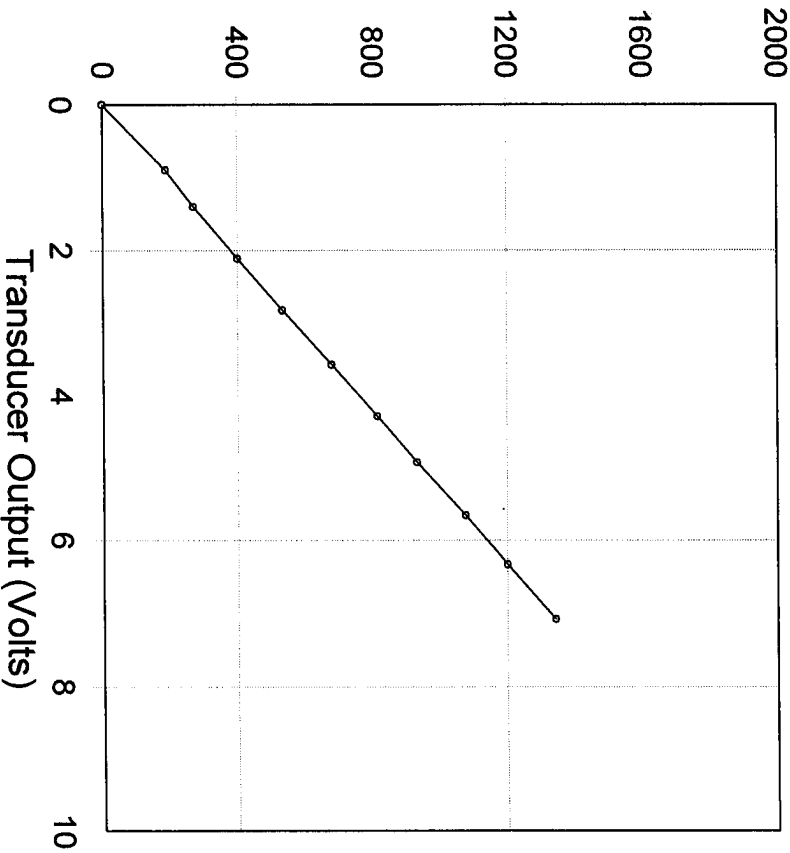

PDA Cal Factor (5.0 V)


94.6 $\mu\epsilon$ /V

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
186	0.90
269	1.41
400	2.11
532	2.81
676	3.56
814	4.28
930	4.92
1074	5.65
1201	6.33
1344	7.07

Shunt (60.4 K Ω) 2.5 V
General Factor 328.3 $\mu\epsilon$ /mV/V

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2011 Version 1.5

Calibrated by: 
Calibrated on: 18-Apr-2014