




Pile Dynamics, Inc.

Transducer C133

Strain ($\mu\epsilon$)

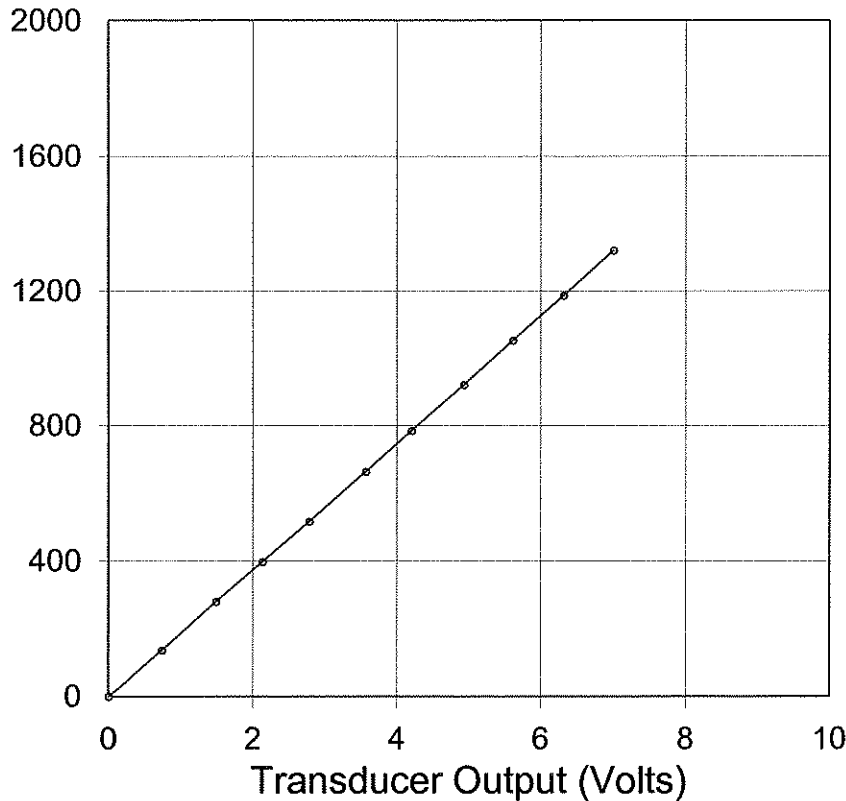

PDA Cal Factor (5.0 V)

94.1 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
138	0.73
280	1.48
398	2.13
517	2.78
664	3.56
784	4.20
922	4.93
1053	5.61
1186	6.31
1322	7.00

Shunt (60.4 K Ω)

2.5 V

General Factor

326.7 $\mu\epsilon/mV/V$

Calibrated by:

Shank BE

Calibrated on:

14-May-2008

Traceable to N.I.S.T.