




# Pile Dynamics, Inc.

## Transducer C134

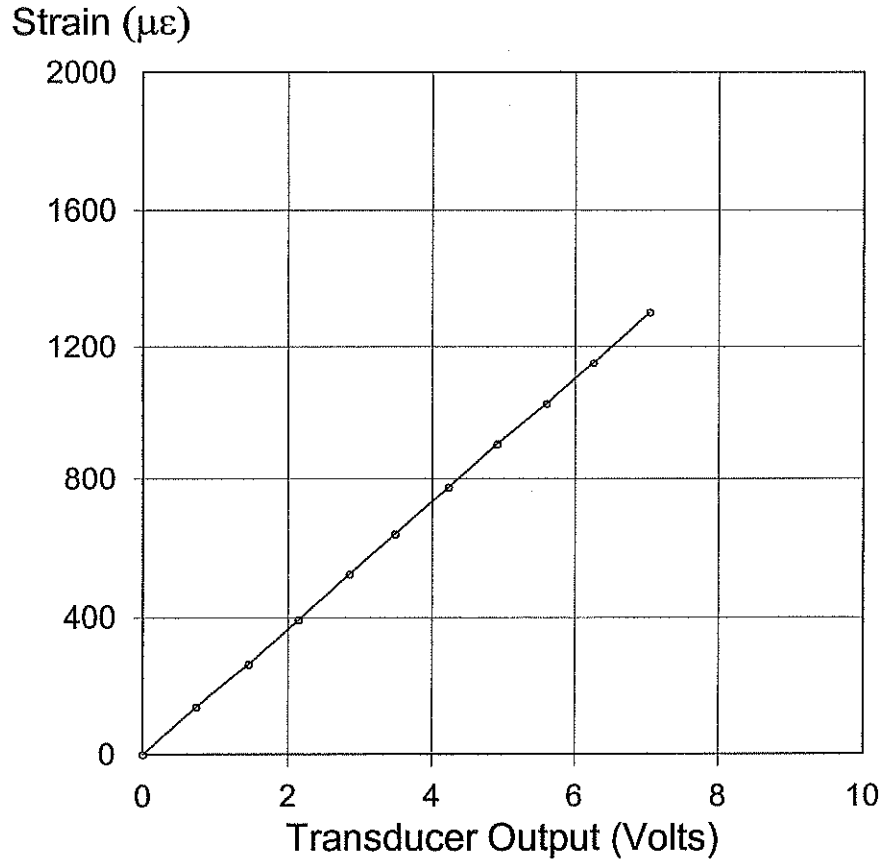

PDA Cal Factor (5.0 V) 92.1  $\mu\epsilon/V$

Applied Strain ( $\mu\epsilon$ )	Transducer Output (Volts)
0	0.00
141	0.73
266	1.45
393	2.14
522	2.85
638	3.48
774	4.22
903	4.90
1026	5.59
1151	6.25
1303	7.04

Shunt (60.4 K $\Omega$ ) 2.5 V  
 General Factor 319.9  $\mu\epsilon/mV/V$

Calibrated by: *Shack*  
 Calibrated on: 22-Jan-2008

Traceable to N.I.S.T.