

Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K15104 Temperature: 22.1 °C
 Model: KICHER PR Humidity: 28%
 Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

418.1 mv/5000g
 (83.6 μ v/g)
 R²: 0.999948 [Chip programmed]

Ref Acc 1: 85382! Cal on: 24Nov2025
 958 g's/volt
 Ref Acc 2: 85363! Cal on: 14Nov2025
 1000 g's/volt


Operator: William Johnson

William Johnson
 Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: JAN 14 2026

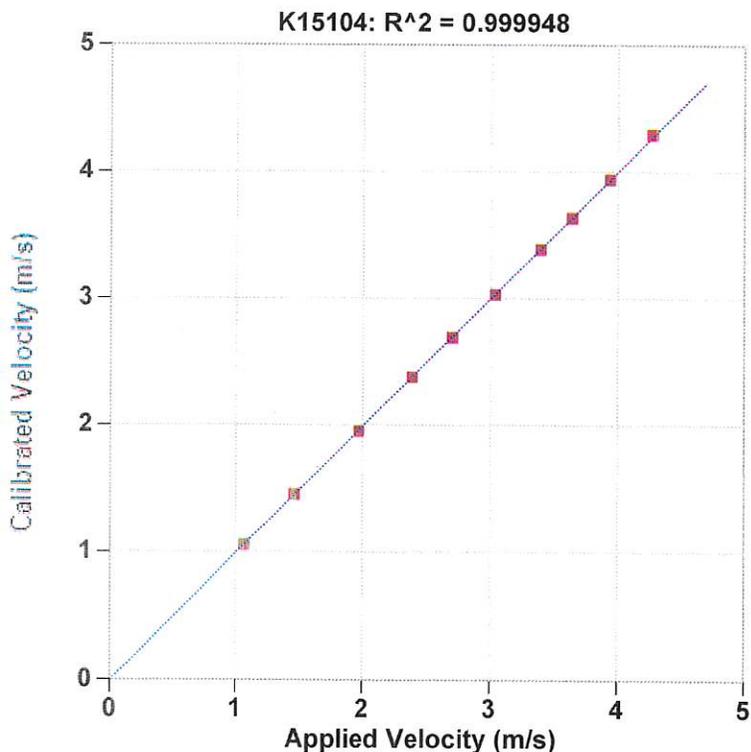

Reference Velocity	S/N K15104 Velocity
m/s	m/s
1.071	1.068
1.462	1.467
1.973	1.963
2.391	2.387
2.707	2.700
3.043	3.038
3.399	3.394
3.645	3.644
3.942	3.945
4.281	4.297
Maximum Acceleration: 923 g's	