


Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

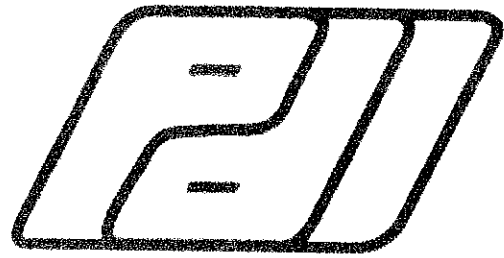

Serial No: K2186 Temperature: 22.3 °C

Model: KICHER PR Humidity: 29%

Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

319.5 mv/5000g


(63.9 μ v/g)

R²: 0.999972 [Chip programmed]

Ref Acc 1: 78268! Cal on: 11Jan2024
986 g's/volt

Ref Acc 2: 78270! Cal on: 11Jan2024
971 g's/volt


Operator: William Johnson

Signed 

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 14Nov2025

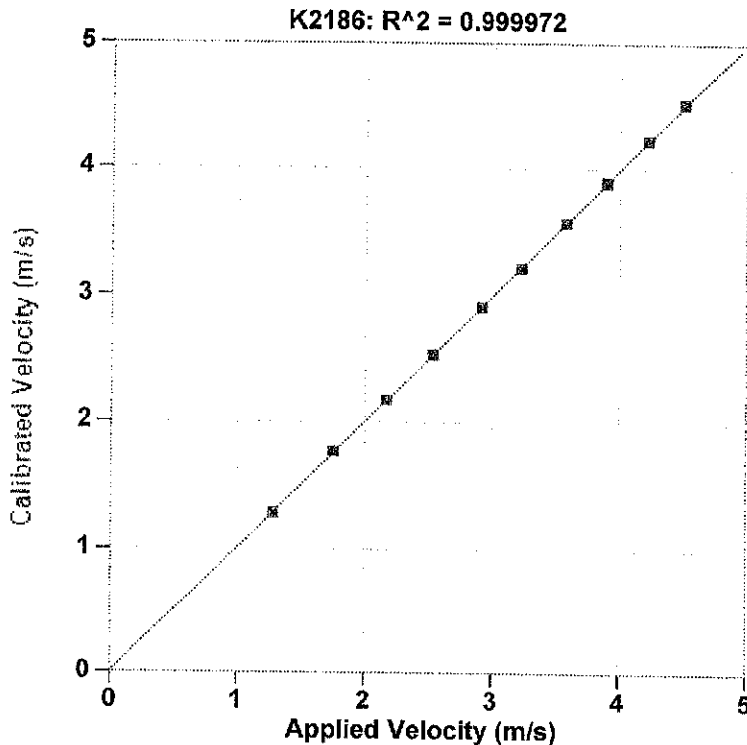

Reference Velocity	S/N K2186 Velocity
m/s	m/s
1.286	1.281
1.755	1.767
2.173	2.176
2.536	2.536
2.918	2.912
3.229	3.222
3.585	3.582
3.901	3.899
4.224	4.227
4.509	4.515
Maximum Acceleration: 978 g's	