


Certificate of Calibration Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

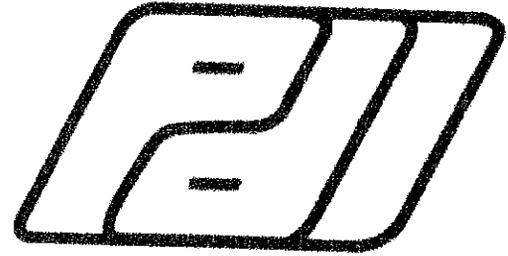

Serial No: K5601 Temperature: 21.9 °C
 Model: KICHER PR Humidity: 27%
 Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR
365.7 mv/5000g
 (73.1 μ v/g)
 R²: 0.999953 [Chip programmed]

Ref Acc 1: 782681 Cal on: 11Jan2024
 986 g's/volt
 Ref Acc 2: 782701 Cal on: 11Jan2024
 971 g's/volt


Operator: William Johnson

William Johnson
 Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 26Dec2025

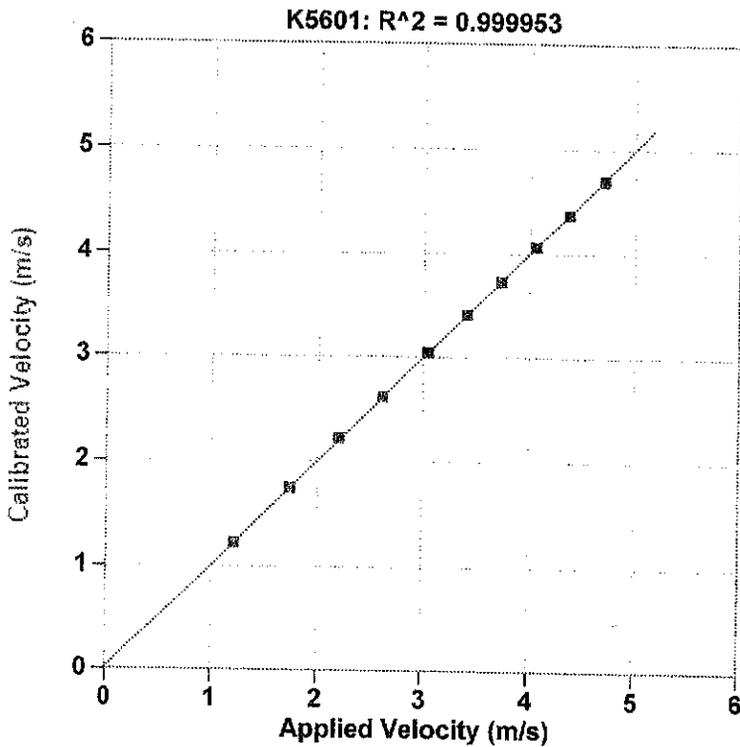

Reference Velocity	S/N K5601 Velocity
m/s	m/s
1.219	1.223
1.745	1.750
2.203	2.221
2.615	2.618
3.046	3.045
3.413	3.410
3.734	3.728
4.064	4.069
4.377	4.375
4.714	4.705

Maximum Acceleration: 1011 g's