




Certificate of Calibration

Pile Dynamics, Inc.
 Transducer Model: PDI Strain Transducer
 Serial Number: 238C
 PDI Gage Factor: 151.0
 Mean Linear Correlation Coefficient: 0.999597

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-2217.8	-4.324	721.8	1.430
-1627.3	-3.149	1069.6	2.083
-1043.3	-2.004	1430.4	2.725
-511.8	-0.960	1791.3	3.369
-164.0	-0.278	2021.0	3.756
269.0	0.555		

Calibration Curve

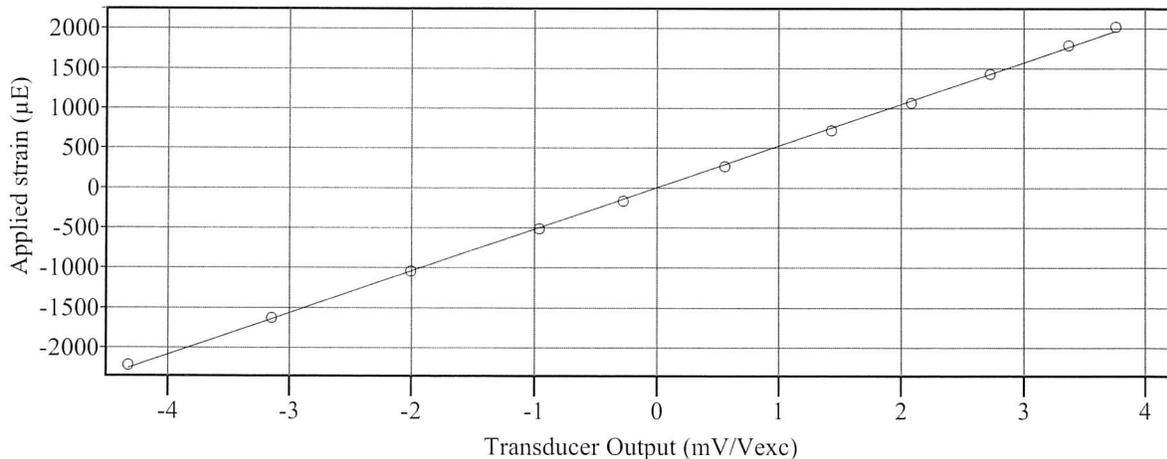

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Kelly Beal
 PDI Gage: 238C
 Calibration Date:

Signature: _____

FEB 25 2026

