




Certificate of Calibration

Pile Dynamics, Inc.
 Transducer Model: PDI Strain Transducer
 Serial Number: 241C
 PDI Gage Factor: 149.0
 Mean Linear Correlation Coefficient: 0.999949

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-2158.8	-4.220	603.7	1.191
-1601.0	-3.122	912.1	1.772
-1036.7	-2.016	1227.0	2.356
-518.4	-1.001	1522.3	2.942
-177.2	-0.339	1850.4	3.571
210.0	0.424	2066.9	3.967

Calibration Curve

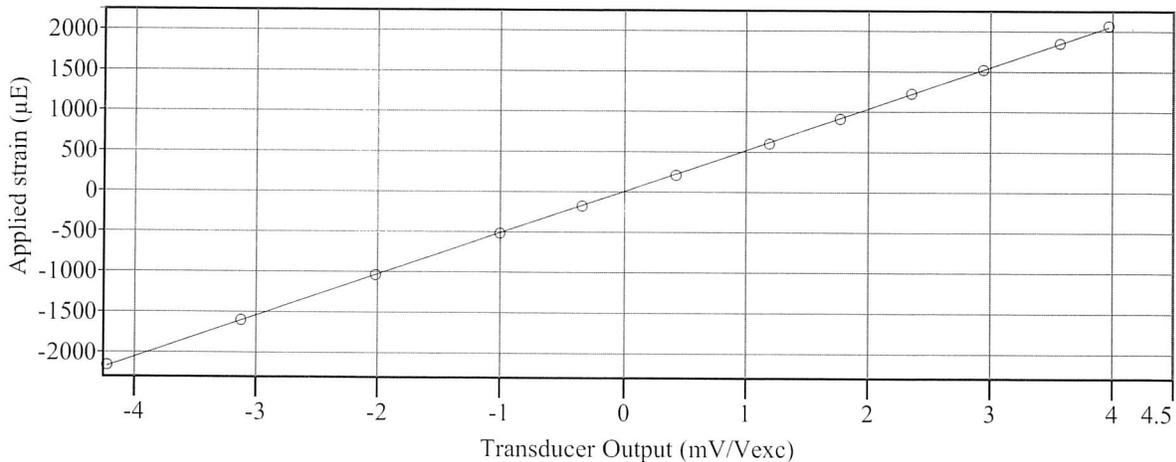

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Kelly Beal
 PDI Gage: 241C
 Calibration Date: _____

Signature: _____

FEB 26 2026

