




# Pile Dynamics, Inc.

## Transducer E723

Strain ( $\mu\epsilon$ )

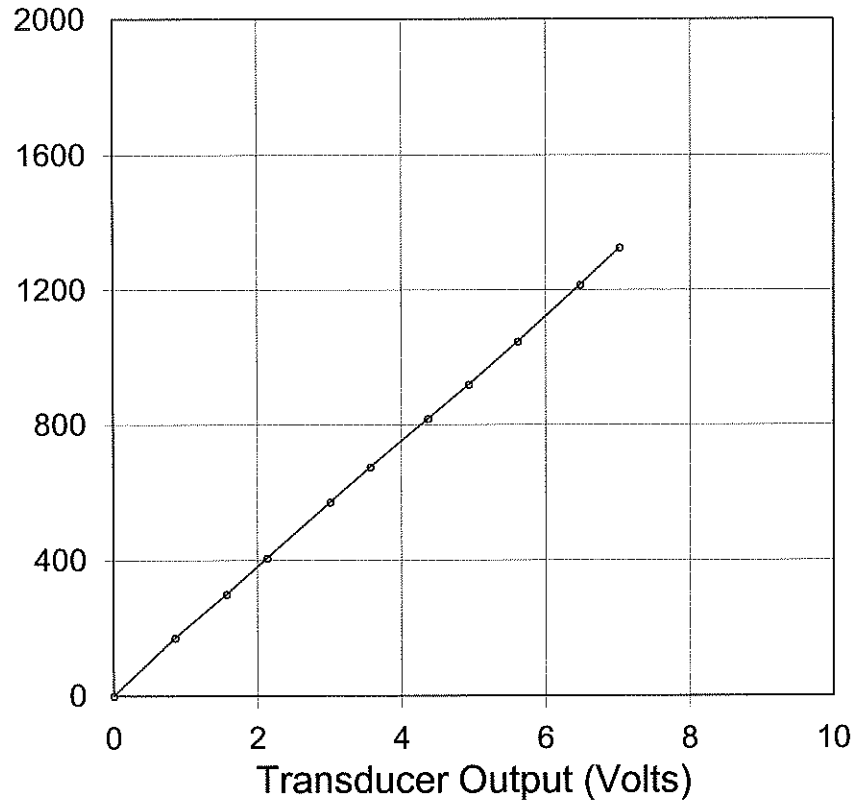

PDA Cal Factor (5.0 V)

93.3 $\mu\epsilon/V$

Applied Strain ( $\mu\epsilon$ )	Transducer Output (Volts)
0	0.00
171	0.84
299	1.56
406	2.13
570	3.00
675	3.57
817	4.37
919	4.93
1047	5.61
1216	6.47
1325	7.02

Shunt (60.4 K $\Omega$ )

2.5 V

General Factor

324.0 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Calibrated by:

Calibrated on:

16-Apr-2010