




Pile Dynamics, Inc.

Transducer E724

Strain ($\mu\epsilon$)

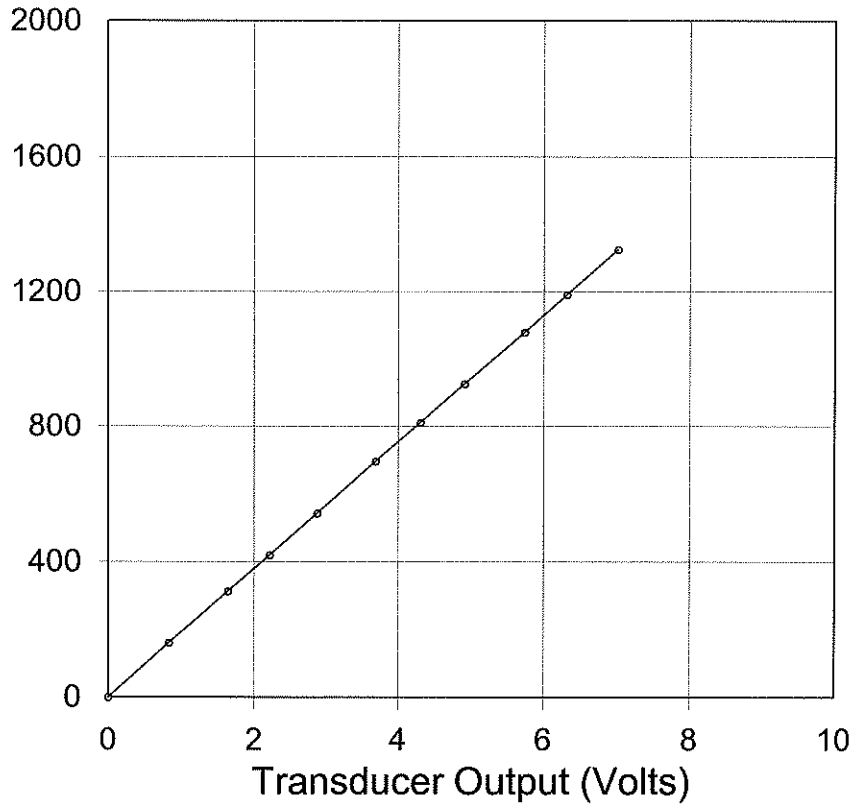

PDA Cal Factor (5.0 V)

94.1 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
162	0.82
312	1.63
420	2.21
543	2.87
696	3.69
810	4.30
926	4.91
1079	5.73
1191	6.31
1325	7.01

Shunt (60.4 K Ω)

2.5 V

General Factor

326.7 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Calibrated by: 

Calibrated on:

16-Apr-2010