


# Pile Dynamics, Inc.

## Transducer E726

Strain ( $\mu\epsilon$ )

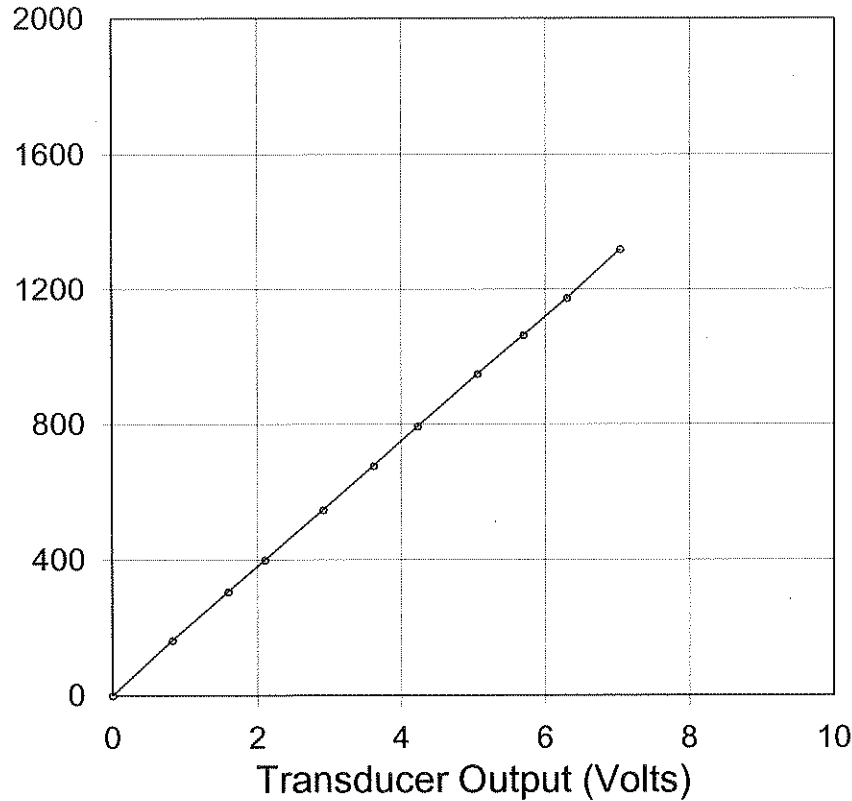

PDA Cal Factor (5.0 V)

93.1  $\mu\epsilon/V$

Applied Strain ( $\mu\epsilon$ )	Transducer Output (Volts)
0	0.00
162	0.82
306	1.59
400	2.10
546	2.92
677	3.62
793	4.23
949	5.05
1063	5.69
1175	6.30
1319	7.04

Shunt (60.4 K $\Omega$ )

2.5 V

General Factor

323.1  $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2009 Version 1.3

Calibrated by:

*Utah*

Calibrated on:

11-Mar-2010

Smart Sensor?  yes  no Smart Chip programmed by: UT on: 3-12-10 CRC value: 2FD7