




Pile Dynamics, Inc.

Transducer E735

Strain ($\mu\epsilon$)

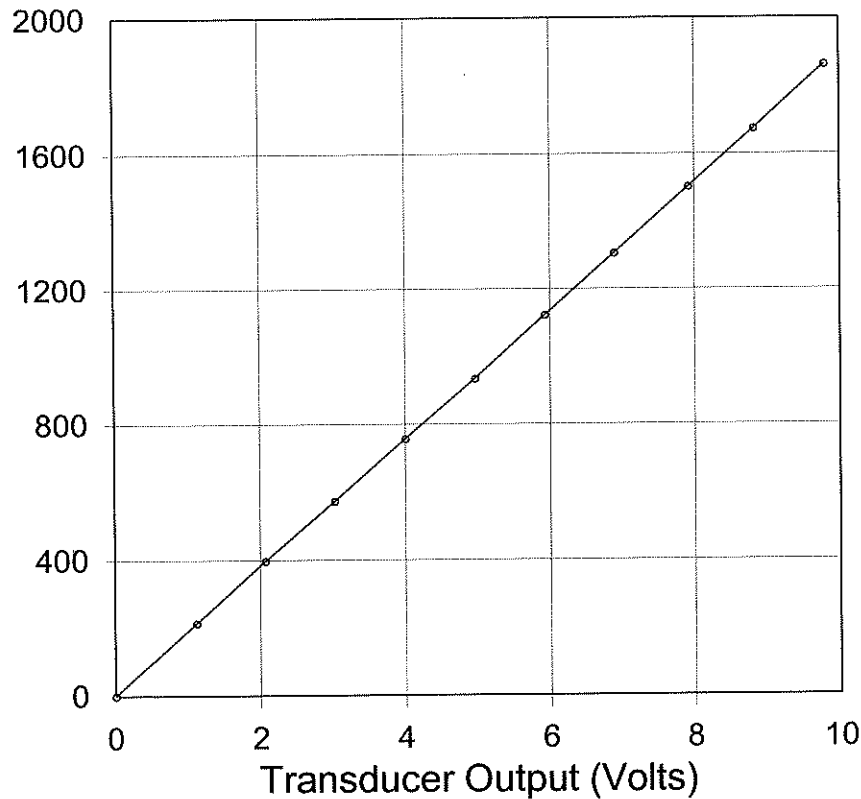

PDA Cal Factor (5.0 V)

94.8 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
216	1.11
398	2.06
573	3.02
755	3.99
933	4.96
1122	5.93
1306	6.89
1504	7.92
1675	8.83
1864	9.80

Shunt (60.4 K Ω)

2.5 V

General Factor

329.1 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Calibrated by: *Cathy Pinnett*

Calibrated on: 30-Apr-2010