




Pile Dynamics, Inc.

Transducer E737

Strain ($\mu\epsilon$)

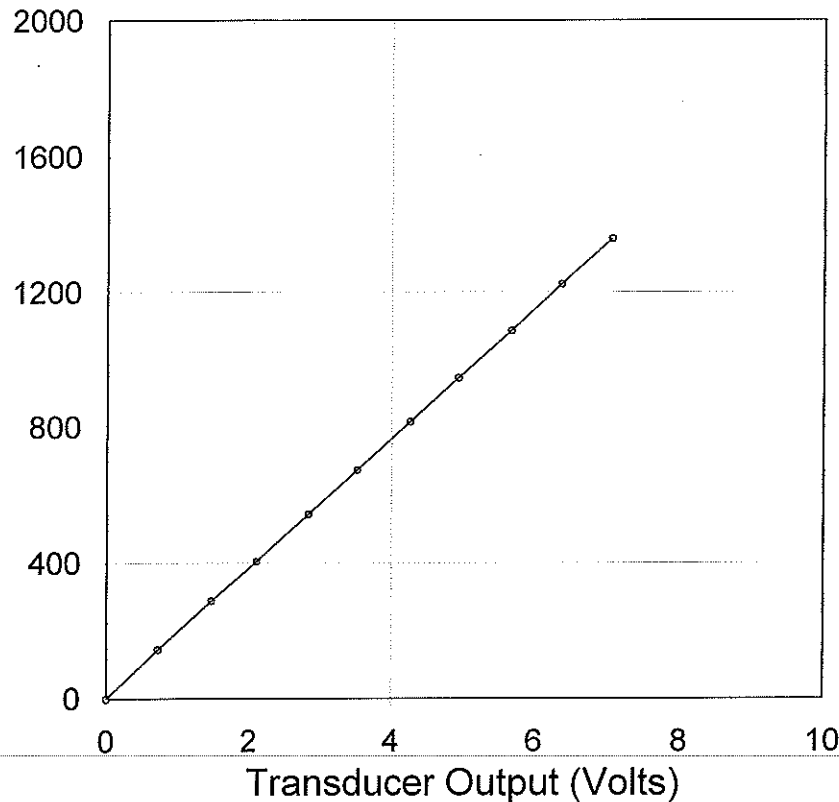

PDA Cal Factor (5.0 V)

95.8 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
147	0.72
289	1.46
403	2.10
541	2.83
671	3.51
816	4.26
945	4.93
1086	5.66
1224	6.36
1359	7.06

Shunt (60.4 K Ω)

2.5 V

General Factor

332.6 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2011 Version 1.5

Calibrated by:

Calibrated on:

12-Aug-2013