




# Pile Dynamics, Inc.

## Transducer E741

Strain ( $\mu\epsilon$ )

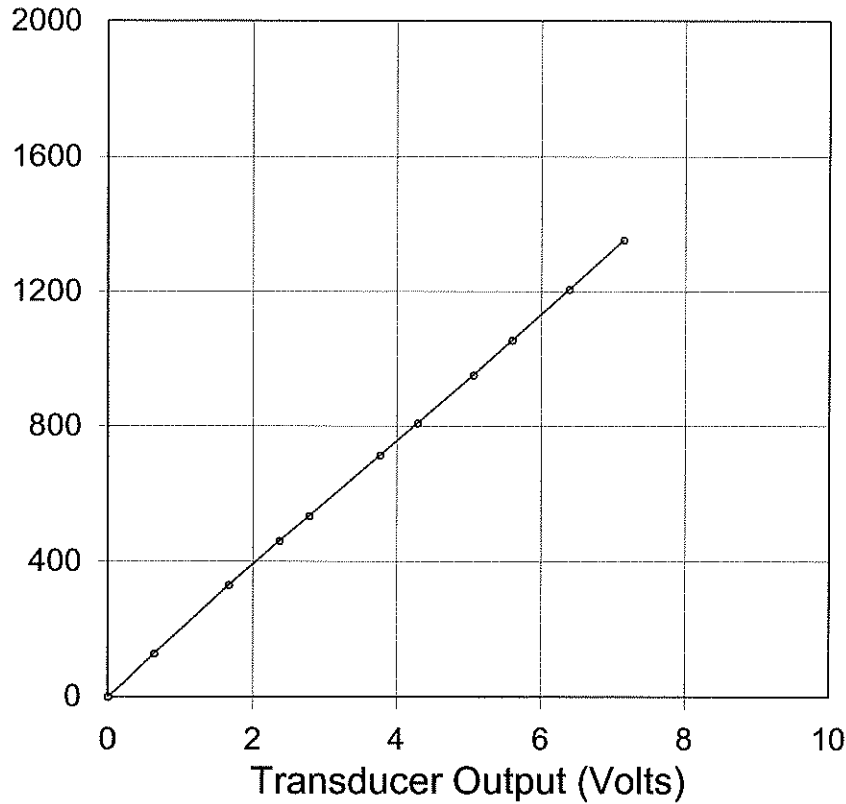

PDA Cal Factor (5.0 V)

93.8 $\mu\epsilon/V$

Applied Strain ( $\mu\epsilon$ )	Transducer Output (Volts)
0	0.00
129	0.63
329	1.66
459	2.37
534	2.78
713	3.76
809	4.28
952	5.05
1054	5.59
1206	6.38
1354	7.14

Shunt (60.4 K $\Omega$ )

2.5 V

General Factor

325.7 $\mu\epsilon/mV/V$

Calibrated by:

Calibrated on:

26-Apr-2010

Traceable to N.I.S.T.