




Pile Dynamics, Inc.

# Pile Dynamics, Inc.

## Transducer E743

Strain ( $\mu\epsilon$ )

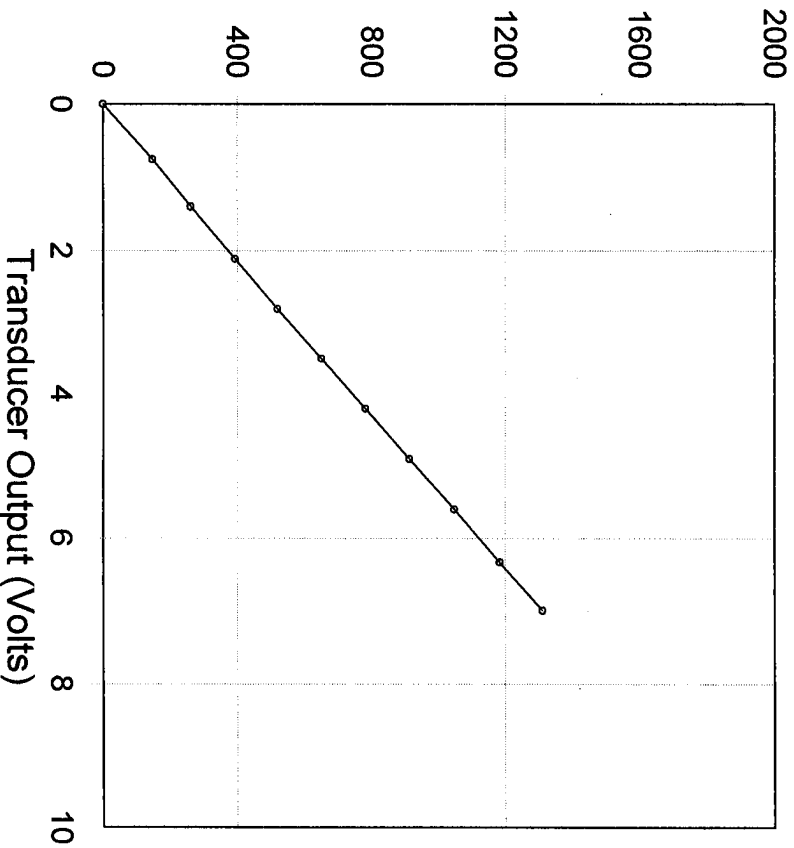

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2011 Version 1.5

PDA Cal Factor (5.0 V)

93.4  $\mu\epsilon/V$

Applied Strain ( $\mu\epsilon$ )	Transducer Output (Volts)
0	0.00
149	0.76
262	1.40
393	2.11
518	2.80
649	3.49
780	4.20
912	4.90
1046	5.60
1183	6.32
1310	6.98

Shunt (60.4 K $\Omega$ )  
General Factor

2.5 V  
324.4  $\mu\epsilon/mV/V$

Calibrated by:

Calibrated on:

20-Oct-2014