




Pile Dynamics, Inc.

Pile Dynamics, Inc. Transducer E749

Strain ($\mu\epsilon$)

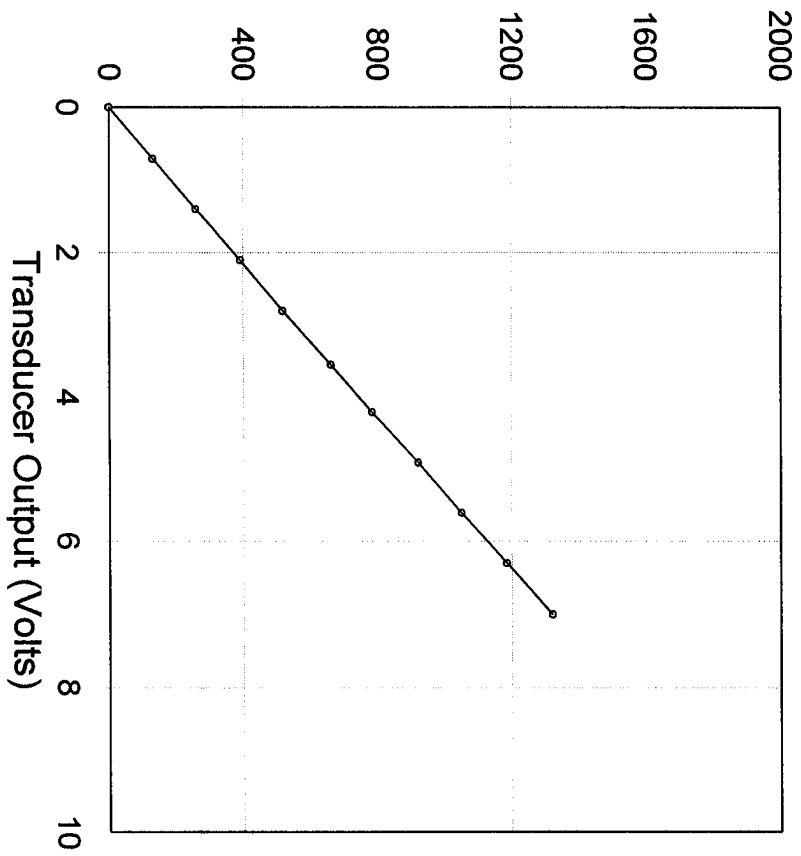

PDA Cal Factor (5.0 V)

94.2 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
132	0.71
259	1.40
390	2.10
516	2.80
659	3.54
783	4.20
919	4.90
1049	5.60
1186	6.30
1320	7.00

Shunt (60.4 K Ω)

2.5 V

General Factor


327.2 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Calibrated by:

Calibrated on:

11-Sep-2014



 11-Sep-2014