




Pile Dynamics, Inc.

Transducer E750

Strain ($\mu\epsilon$)

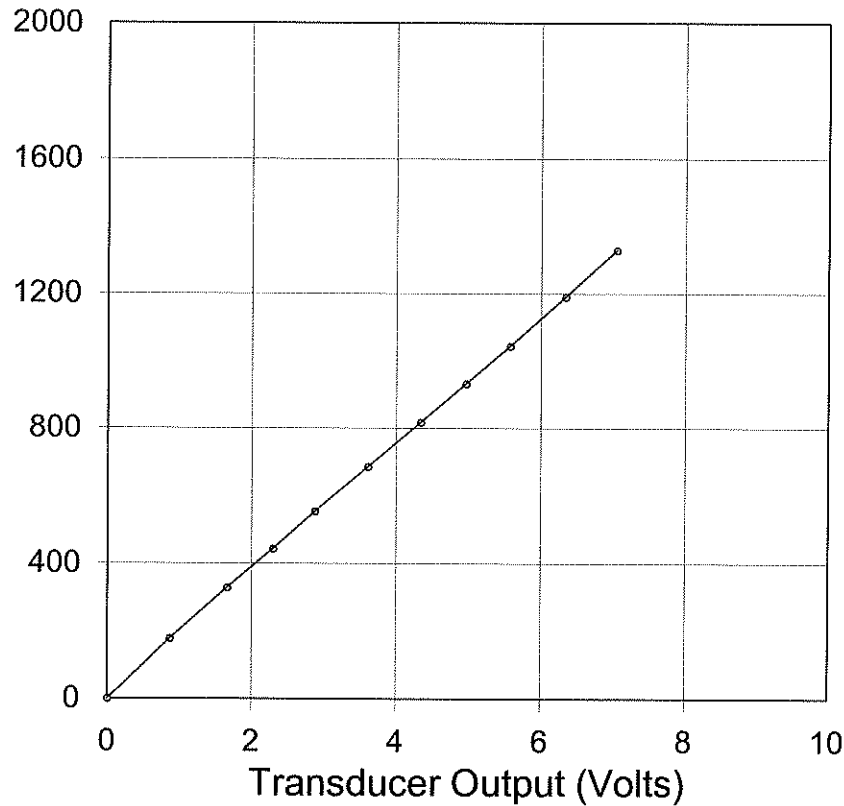

PDA Cal Factor (5.0 V)

93.2 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
178	0.85
329	1.66
443	2.29
552	2.87
685	3.60
817	4.33
931	4.96
1045	5.57
1191	6.33
1330	7.04

Shunt (60.4 K Ω)

2.5 V

General Factor

323.7 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Calibrated by:

Calibrated on:

18-May-2010