




Pile Dynamics, Inc.

Transducer E753

Strain ($\mu\epsilon$)

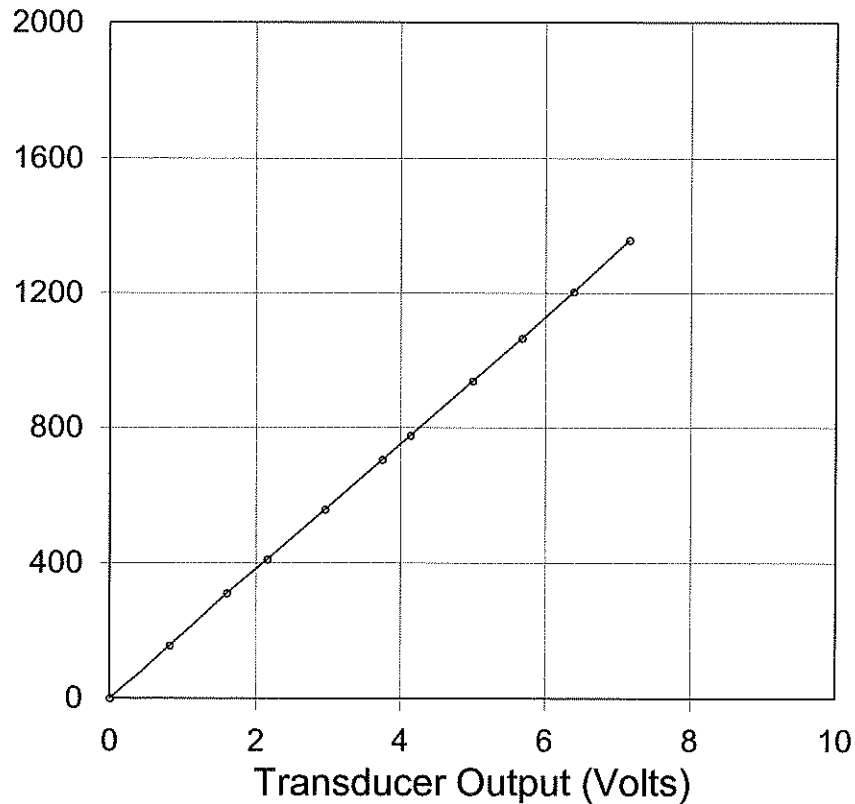

PDA Cal Factor (5.0 V)

94.1 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
157	0.81
310	1.60
411	2.15
557	2.95
705	3.74
776	4.13
938	4.99
1066	5.67
1205	6.38
1358	7.15

Shunt (60.4 K Ω)

2.5 V

General Factor

326.9 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Calibrated by:

Calibrated on:

18-May-2010