




Pile Dynamics, Inc.

Transducer E754

Strain ($\mu\epsilon$)

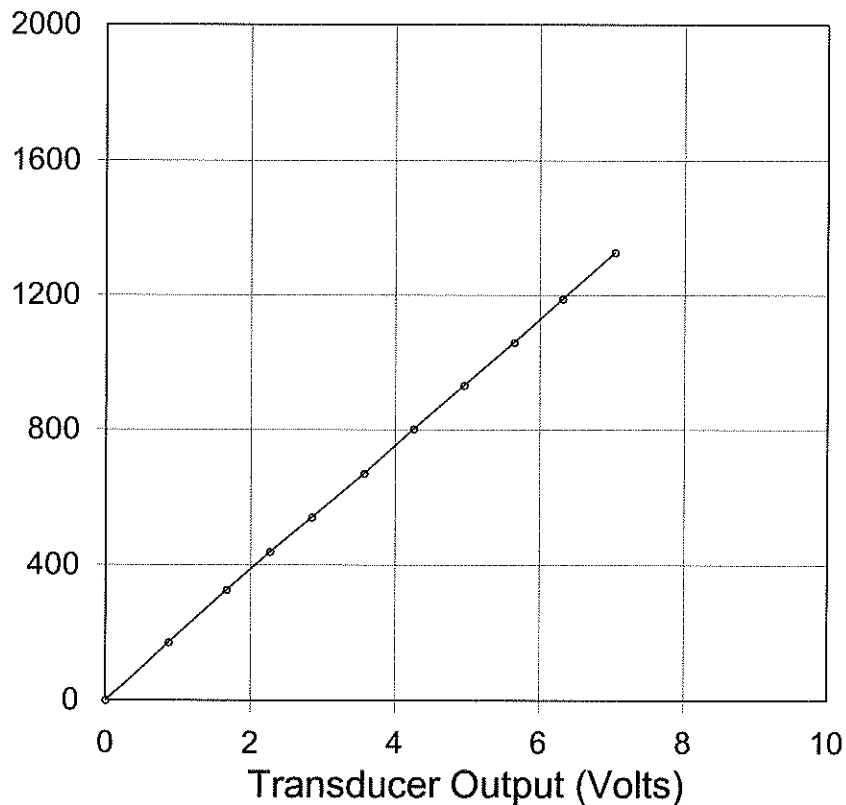

PDA Cal Factor (5.0 V)

93.6 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
171	0.86
326	1.66
438	2.26
541	2.84
671	3.56
801	4.25
931	4.95
1059	5.64
1189	6.31
1328	7.03

Shunt (60.4 K Ω)

2.5 V

General Factor

325.0 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2009 Version 1.3

Calibrated by:

Calibrated on:

[Signature]
18-May-2010