




# Pile Dynamics, Inc.

## Transducer E757

Strain ( $\mu\epsilon$ )

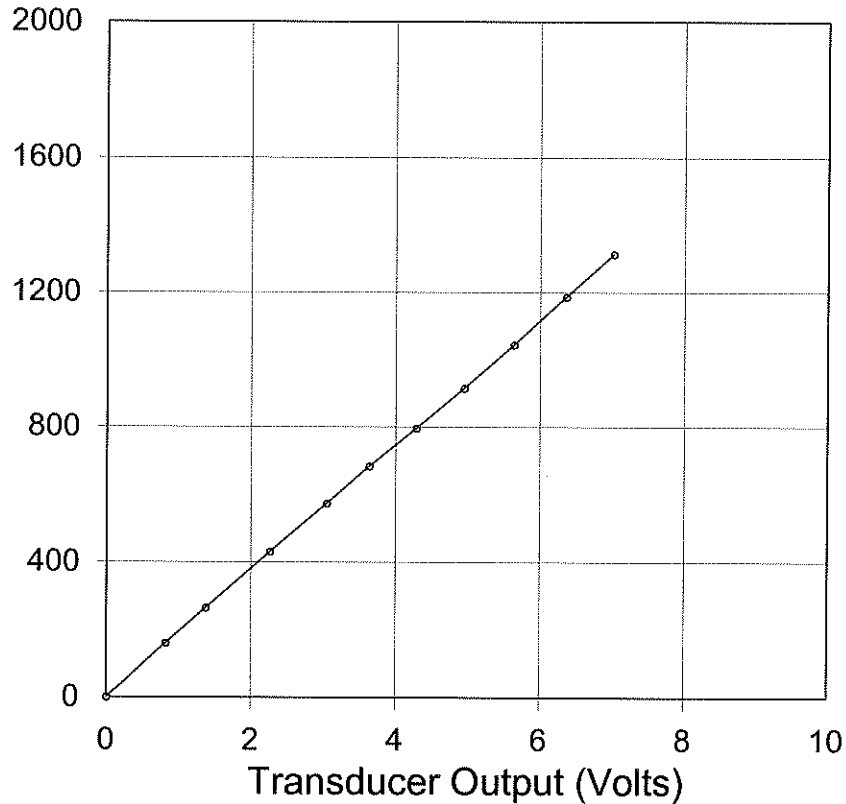

PDA Cal Factor (5.0 V)

92.8 $\mu\epsilon/V$

Applied Strain ( $\mu\epsilon$ )	Transducer Output (Volts)
0	0.00
162	0.81
265	1.37
429	2.27
573	3.04
682	3.64
796	4.28
915	4.94
1045	5.63
1187	6.35
1314	7.01

Shunt (60.4 K $\Omega$ )

2.5 V

General Factor

322.2 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Calibrated by:

Calibrated on:

18-May-2010