




Pile Dynamics, Inc.

Transducer E758

Strain ($\mu\epsilon$)

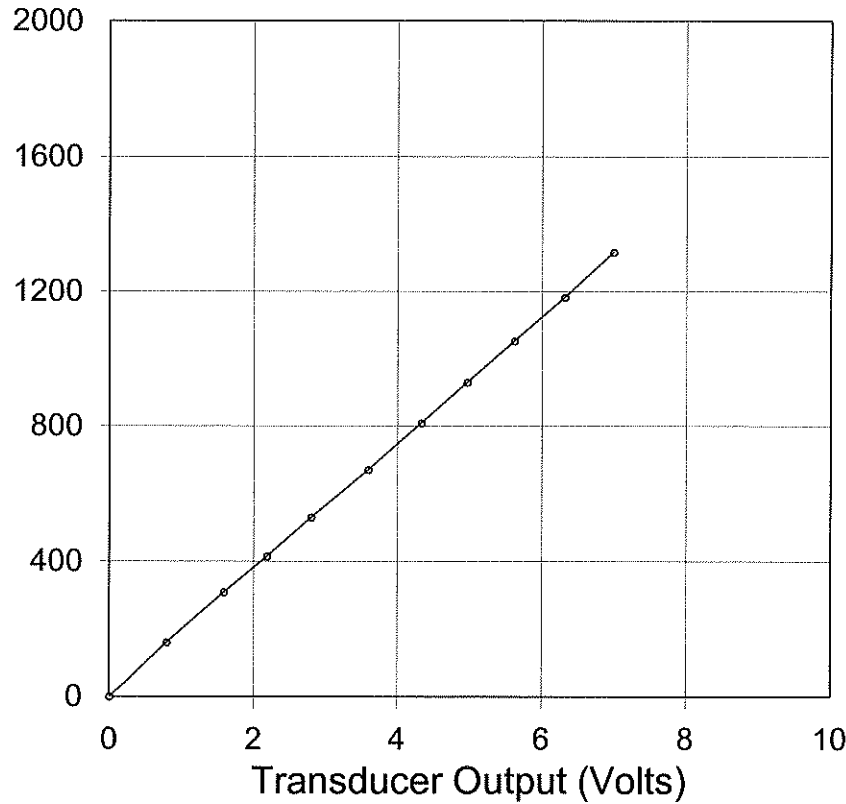

PDA Cal Factor (5.0 V)

93.1 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
162	0.78
308	1.58
415	2.18
529	2.80
671	3.59
808	4.32
929	4.96
1052	5.61
1182	6.31
1317	6.99

Shunt (60.4 K Ω)

2.5 V

General Factor

323.4 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2009 Version 1.3

Calibrated by:

Calibrated on:

Stack
18-May-2010