




Pile Dynamics, Inc.

Pile Dynamics, Inc.

Transducer

E760

Strain ($\mu\epsilon$)

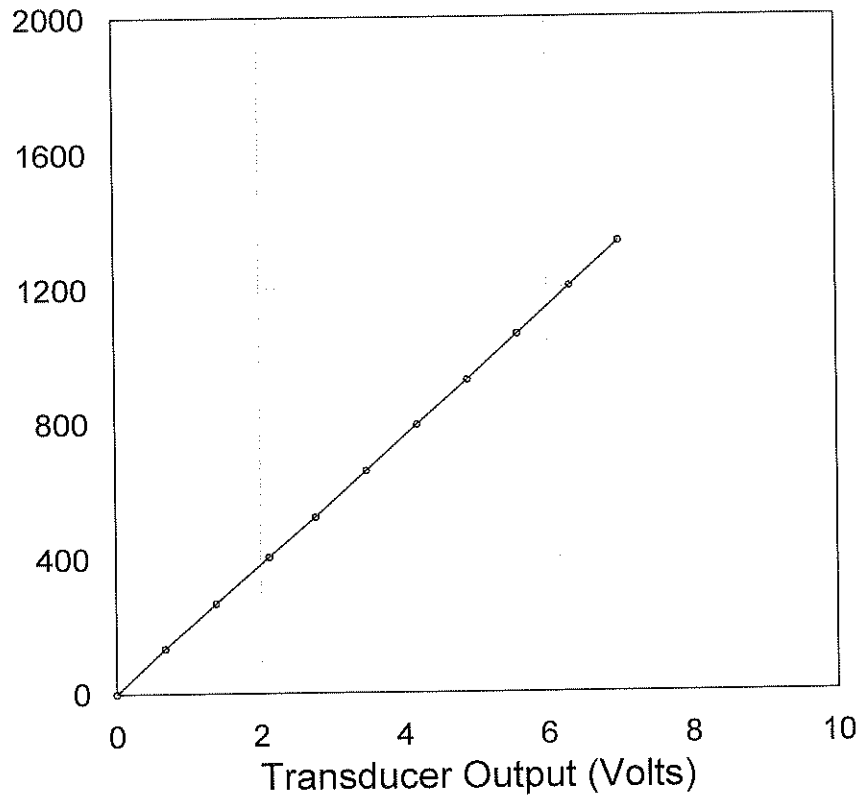

PDA Cal Factor (5.0 V)

94.9 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
135	0.67
266	1.38
404	2.11
521	2.77
657	3.48
792	4.19
925	4.89
1061	5.59
1206	6.32
1337	7.00

Shunt (60.4 K Ω)

2.5 V

General Factor

329.7 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Calibrated by:

Calibrated on:

29-Dec-2011