




# Pile Dynamics, Inc.

## Transducer E762

Strain ( $\mu\epsilon$ )

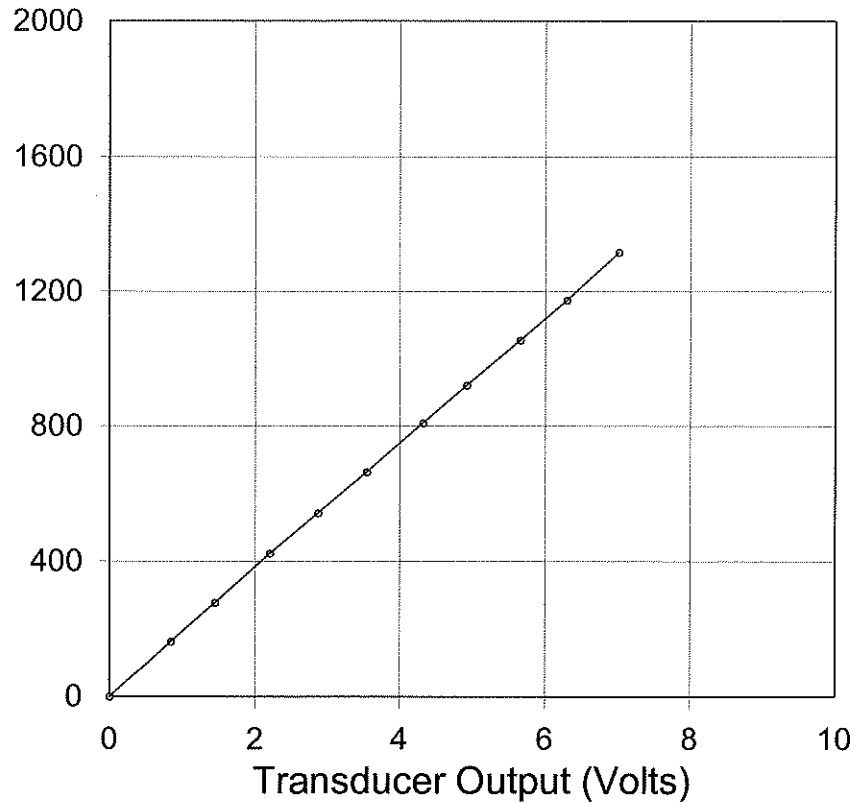

PDA Cal Factor (5.0 V)

93.1 $\mu\epsilon/V$

Applied Strain ( $\mu\epsilon$ )	Transducer Output (Volts)
0	0.00
164	0.83
277	1.44
423	2.20
543	2.87
663	3.54
808	4.31
921	4.92
1055	5.65
1175	6.29
1316	7.01

Shunt (60.4 K $\Omega$ )

2.5 V

General Factor

323.3 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Calibrated by:

Calibrated on:

30-Jul-2010