




Pile Dynamics, Inc.

Transducer E765

Strain ($\mu\epsilon$)

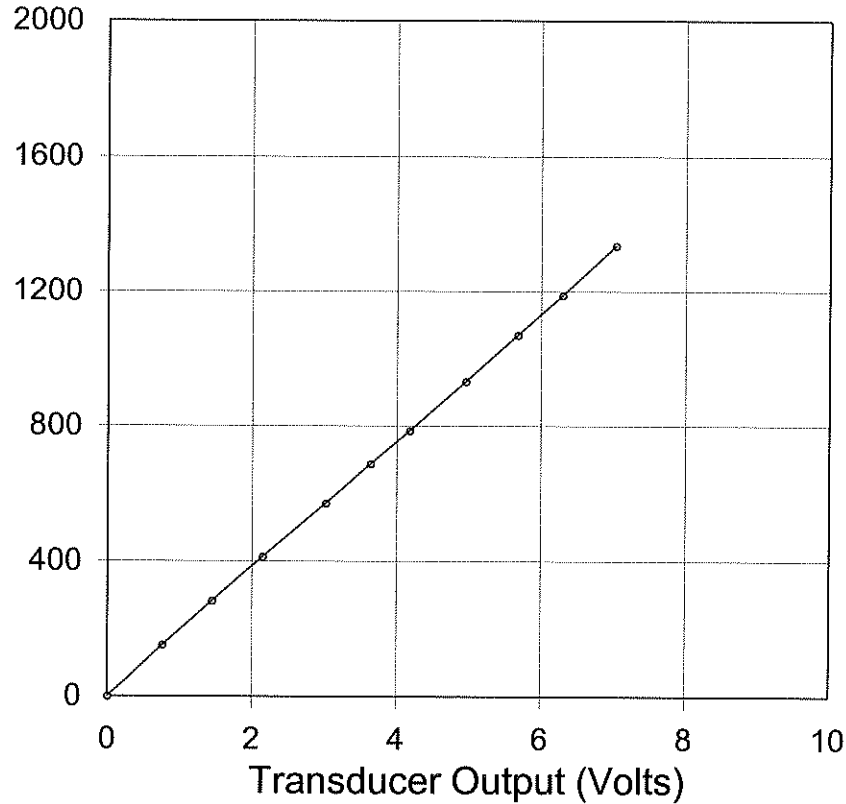

PDA Cal Factor (5.0 V)

94.1 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
153	0.75
283	1.44
413	2.14
571	3.01
687	3.63
785	4.17
931	4.95
1070	5.67
1189	6.29
1337	7.03

Shunt (60.4 K Ω)

2.5 V

General Factor

326.6 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Calibrated by:

Calibrated on:

18-May-2010