




Pile Dynamics, Inc.

Transducer E767

Strain ($\mu\epsilon$)

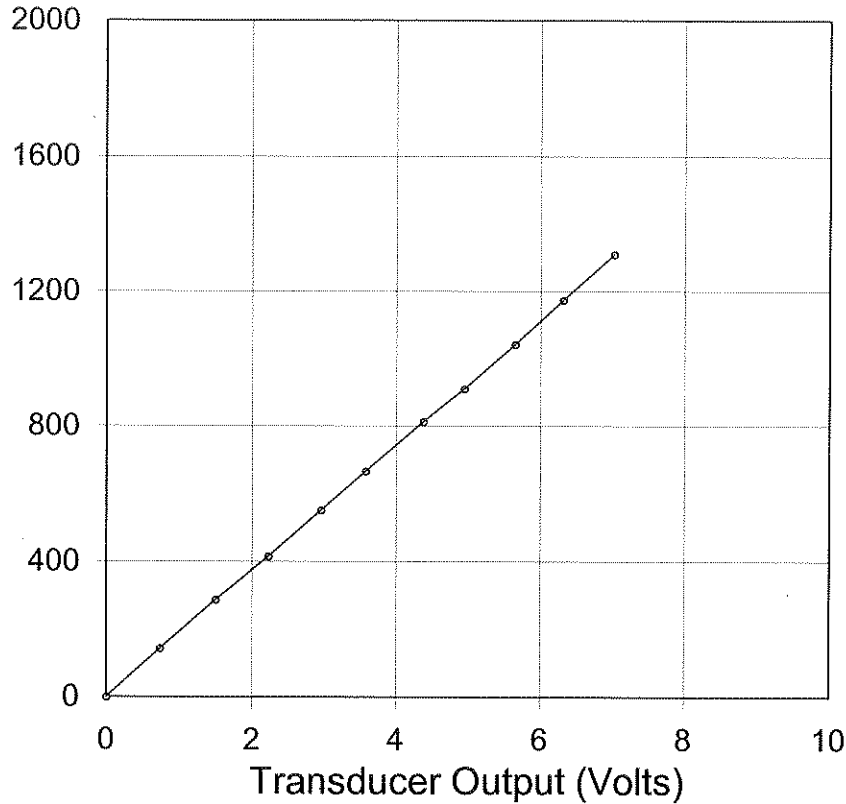

PDA Cal Factor (5.0 V)

92.6 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
143	0.73
287	1.50
414	2.22
551	2.95
665	3.57
813	4.38
911	4.94
1043	5.64
1175	6.31
1311	7.02

Shunt (60.4 K Ω)

2.5 V

General Factor

321.4 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2009 Version 1.3

Calibrated by: *Chau*

Calibrated on: 24-Mar-2010

Smart Sensor? yes no Smart Chip programmed by: VT on: 3-25-10 CRC value: E041