




Pile Dynamics, Inc.

Transducer E768

Strain ($\mu\epsilon$)

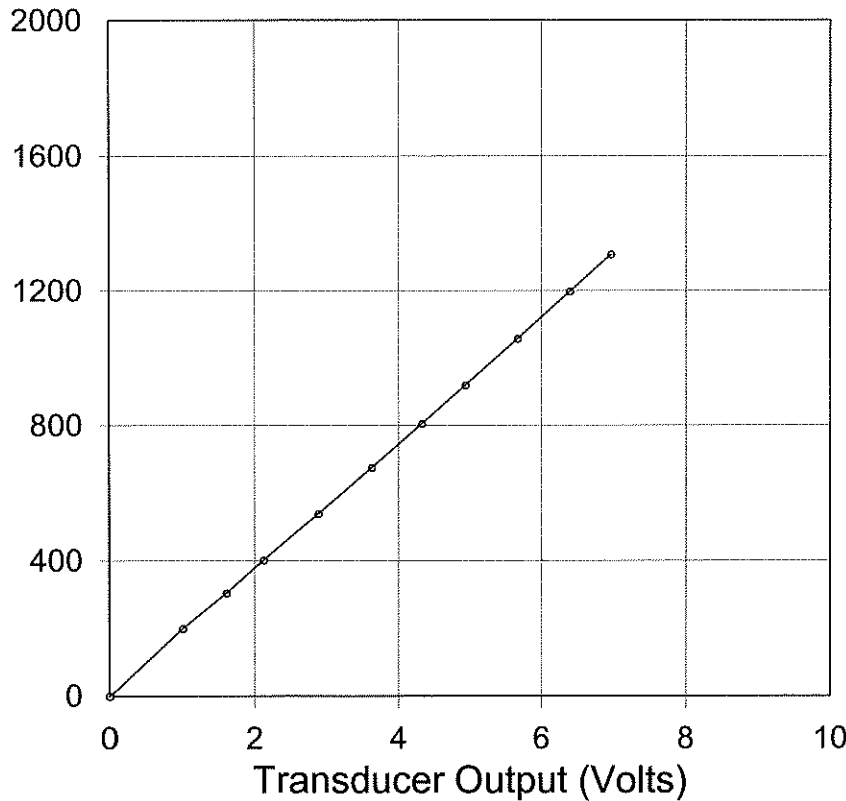

PDA Cal Factor (5.0 V)

93.2 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
200	1.00
304	1.60
402	2.12
538	2.88
675	3.62
804	4.32
918	4.93
1056	5.67
1197	6.39
1309	6.95

Shunt (60.4 K Ω)

2.5 V

General Factor

323.5 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Calibrated by:

Calibrated on:

26-Apr-2010