




Pile Dynamics, Inc.

Transducer E772

Strain ($\mu\epsilon$)

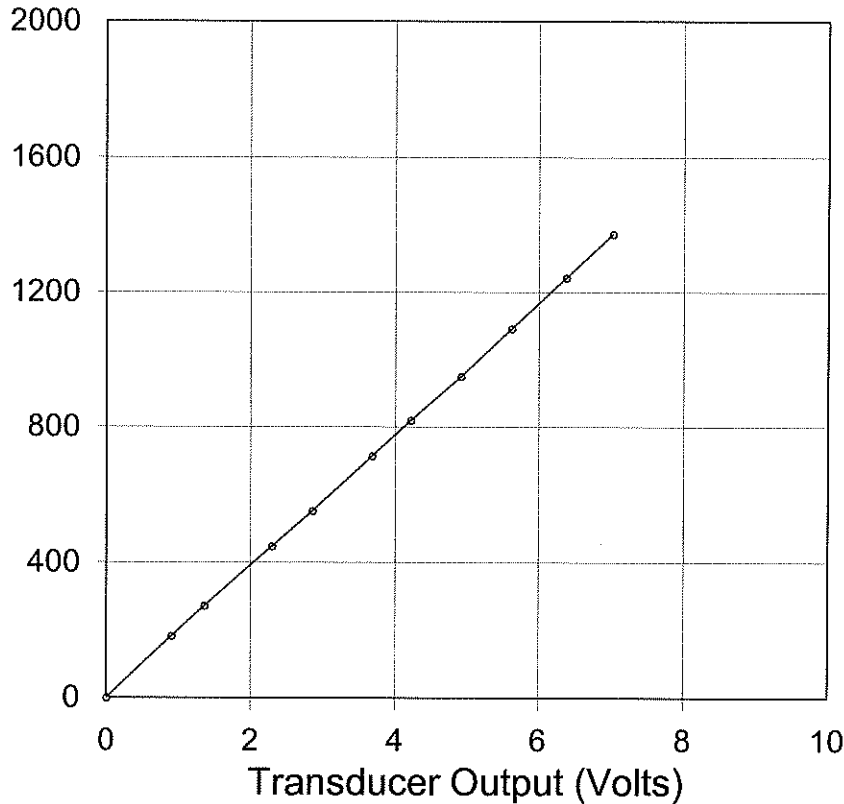

PDA Cal Factor (5.0 V)

97.2 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
184	0.89
271	1.35
448	2.30
551	2.85
714	3.67
820	4.21
948	4.91
1093	5.62
1244	6.37
1373	7.02

Shunt (60.4 K Ω)

2.5 V

General Factor

337.3 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Calibrated by:

Handwritten signature

Calibrated on:

03-Mar-2010