




Pile Dynamics, Inc.

Transducer E773

Strain ($\mu\epsilon$)

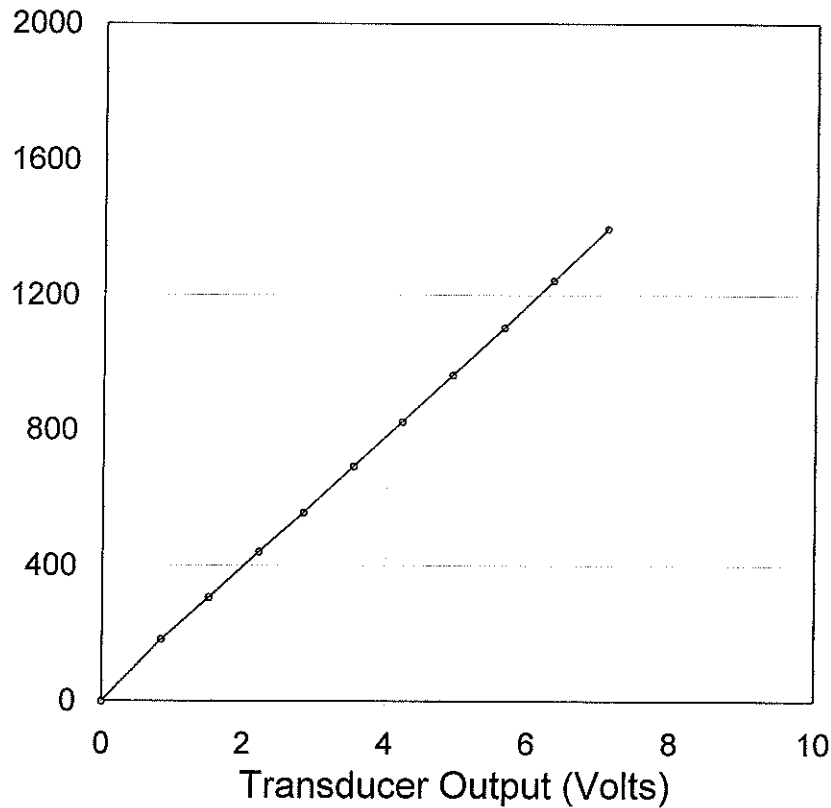

PDA Cal Factor (5.0 V)

97.7 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
183	0.84
307	1.51
441	2.21
555	2.83
692	3.53
823	4.21
963	4.91
1103	5.63
1243	6.32
1398	7.08

Shunt (60.4 K Ω)

2.5 V

General Factor

339.3 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2011 Version 1.5

Calibrated by:

Calibrated on:

25-Jun-2013