




# Pile Dynamics, Inc.

## Transducer E775

Strain ( $\mu\epsilon$ )

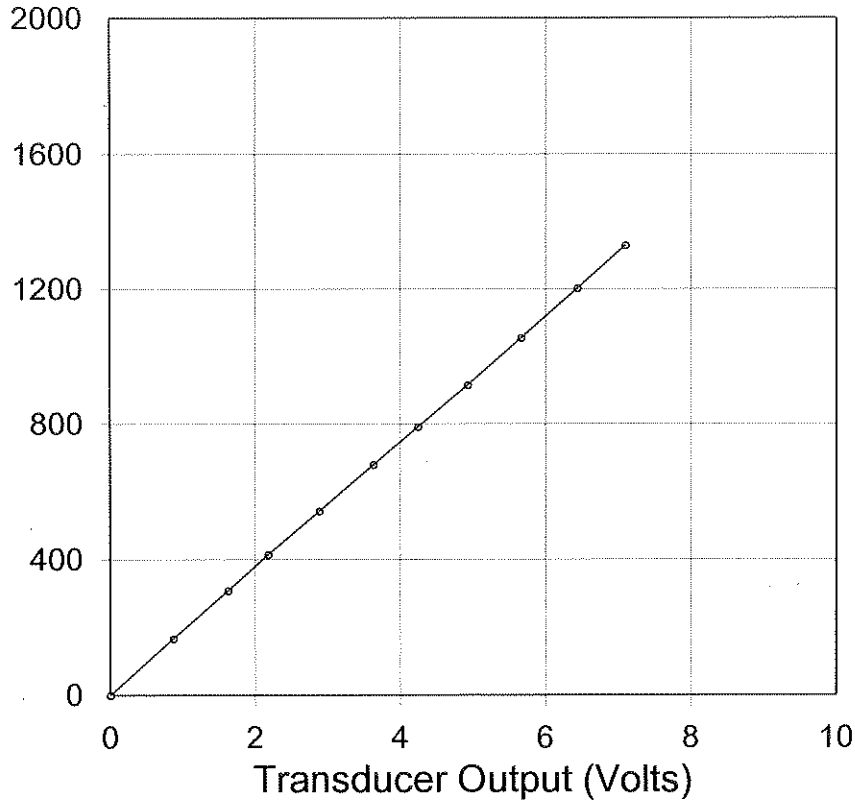

PDA Cal Factor (5.0 V)

93.1 $\mu\epsilon/V$

Applied Strain ( $\mu\epsilon$ )	Transducer Output (Volts)
0	0.00
168	0.86
308	1.62
414	2.18
542	2.89
678	3.63
791	4.24
915	4.92
1055	5.66
1202	6.43
1331	7.10

Shunt (60.4 K $\Omega$ )

2.5 V

General Factor

323.2 $\mu\epsilon/mV/V$

Calibrated by: *Strack*

Calibrated on: 23-Feb-2010

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2009 Version 1.3

Smart Sensor?  yes  no Smart Chip programmed by: VT on: 2-23-10 CRC value: 355F