




Pile Dynamics, Inc.

Transducer E777

Strain ($\mu\epsilon$)

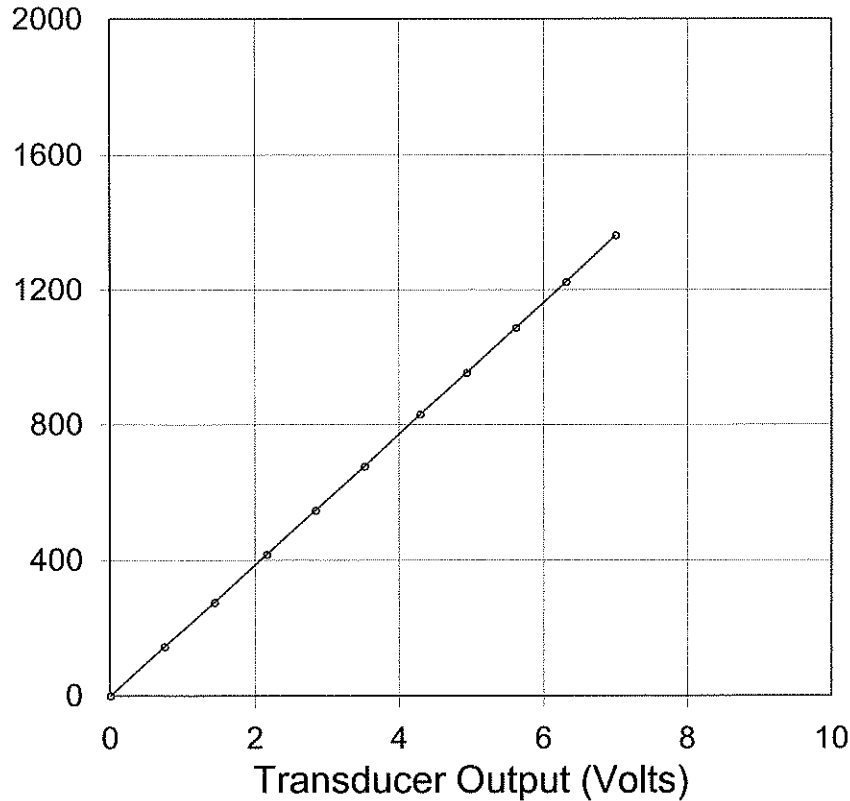

PDA Cal Factor (5.0 V)

97.1 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
145	0.74
275	1.43
416	2.16
546	2.84
677	3.52
830	4.29
953	4.93
1087	5.61
1223	6.31
1362	7.00

Shunt (60.4 K Ω)

2.5 V

General Factor

337.0 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Calibrated by:

Keith Asstn

Calibrated on:

21-Dec-2009