


Pile Dynamics, Inc.

Transducer E779

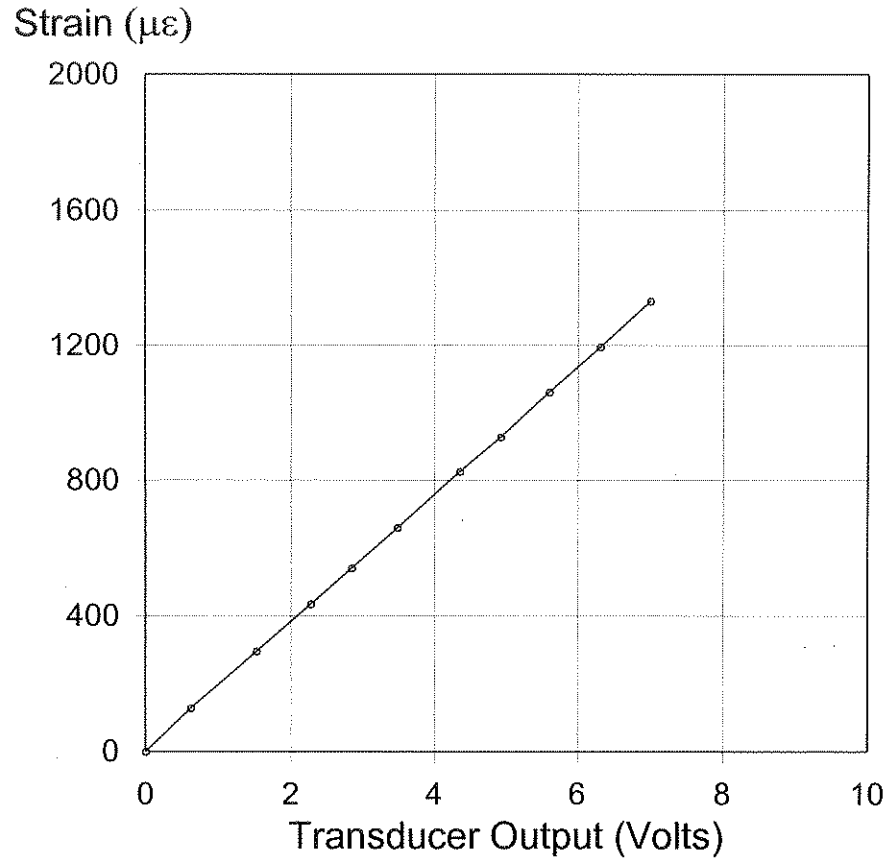

PDA Cal Factor (5.0 V) 94.4 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
128	0.62
296	1.52
433	2.28
541	2.84
660	3.48
825	4.35
928	4.92
1061	5.60
1196	6.31
1331	7.00

Shunt (60.4 K Ω) 2.5 V
 General Factor 327.7 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2009 Version 1.3

Calibrated by: *Strick*
 Calibrated on: 08-Feb-2010

Smart Sensor? yes no Smart Chip programmed by: VT on: 2-8-10 CRC value: 098C