




Pile Dynamics, Inc.

Transducer E793

Strain ($\mu\epsilon$)

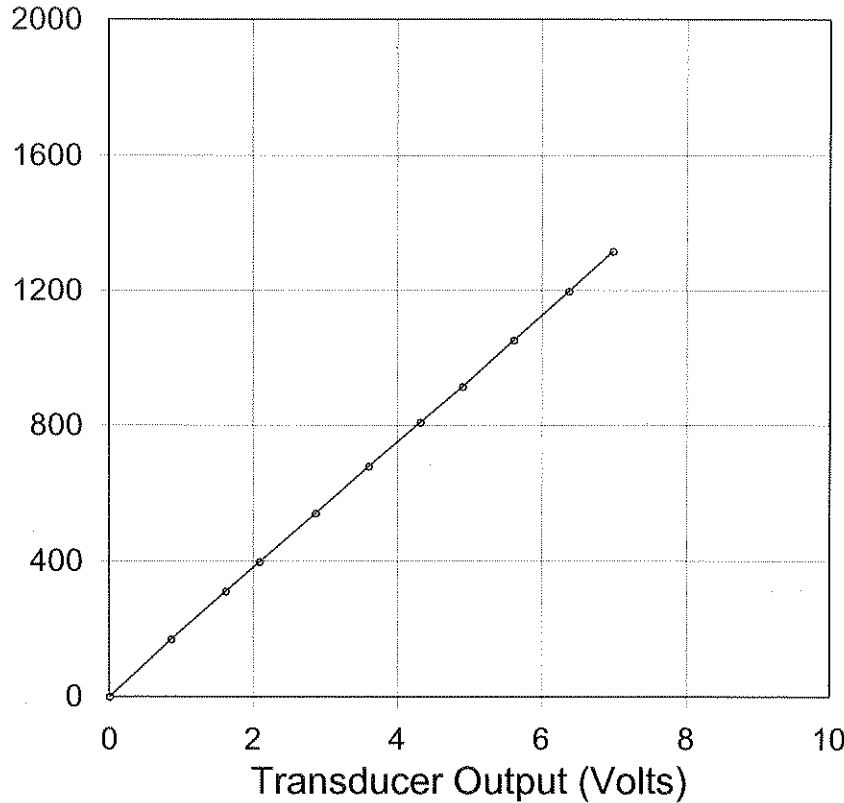

PDA Cal Factor (5.0 V)

93.6 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
170	0.85
312	1.62
396	2.09
541	2.87
678	3.61
809	4.31
914	4.90
1054	5.61
1198	6.37
1317	6.98

Shunt (60.4 K Ω)

2.5 V

General Factor

325.0 $\mu\epsilon/mV/V$

Calibrated by: *Utach*

Calibrated on:

08-Feb-2010

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2009 Version 1.3

Smart Sensor? yes no Smart Chip programmed by: UT on: 2-8-10 CRC value: 5DF7