




Pile Dynamics, Inc.

# Pile Dynamics, Inc.

## Transducer E794

Strain ( $\mu\epsilon$ )

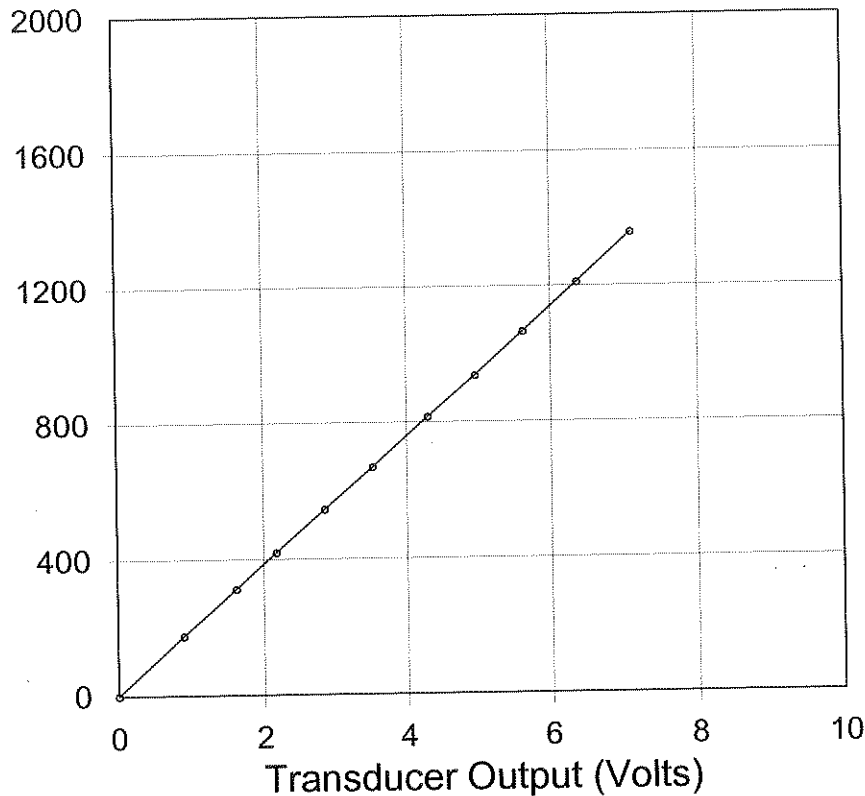

PDA Cal Factor (5.0 V)

94.8 $\mu\epsilon/V$

Applied Strain ( $\mu\epsilon$ )	Transducer Output (Volts)
0	0.00
177	0.88
313	1.62
418	2.17
545	2.85
669	3.52
816	4.29
935	4.95
1066	5.62
1211	6.36
1358	7.11

Shunt (60.4 K $\Omega$ )  
General Factor

2.5 V  
329.3 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2009 Version 1.3

Calibrated by: \_\_\_\_\_  
Calibrated on: \_\_\_\_\_

*Frank*  
23-Feb-2010

Smart Sensor?  yes  no Smart Chip programmed by: VT on: 2-23-10 CRC value: 41E6