




Pile Dynamics, Inc.

Transducer E795

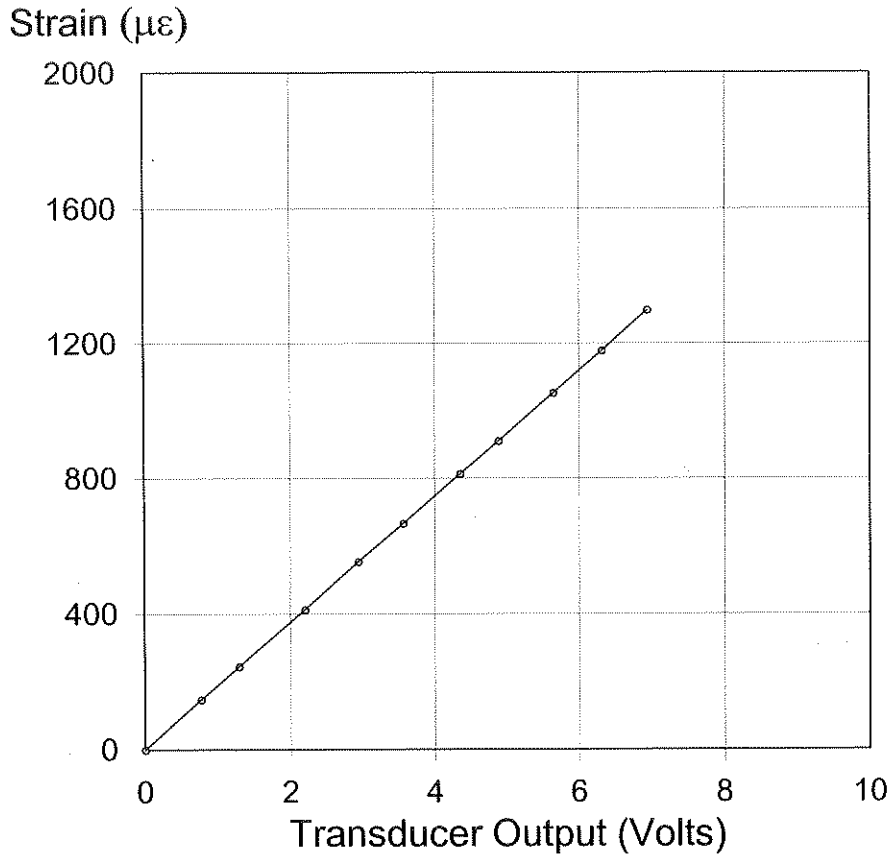

PDA Cal Factor (5.0 V) 93.2 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
149	0.77
246	1.29
413	2.20
553	2.94
665	3.56
812	4.35
911	4.88
1053	5.64
1179	6.31
1299	6.94

Shunt (60.4 K Ω) 2.5 V
 General Factor 323.5 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2009 Version 1.3

Calibrated by: *Uthair*
 Calibrated on: 20-Jan-2010

Smart Sensor? yes no Smart Chip programmed by: VT on: 1-20-10 CRC value: 04C0