




Pile Dynamics, Inc.

Transducer E797

Strain ($\mu\epsilon$)

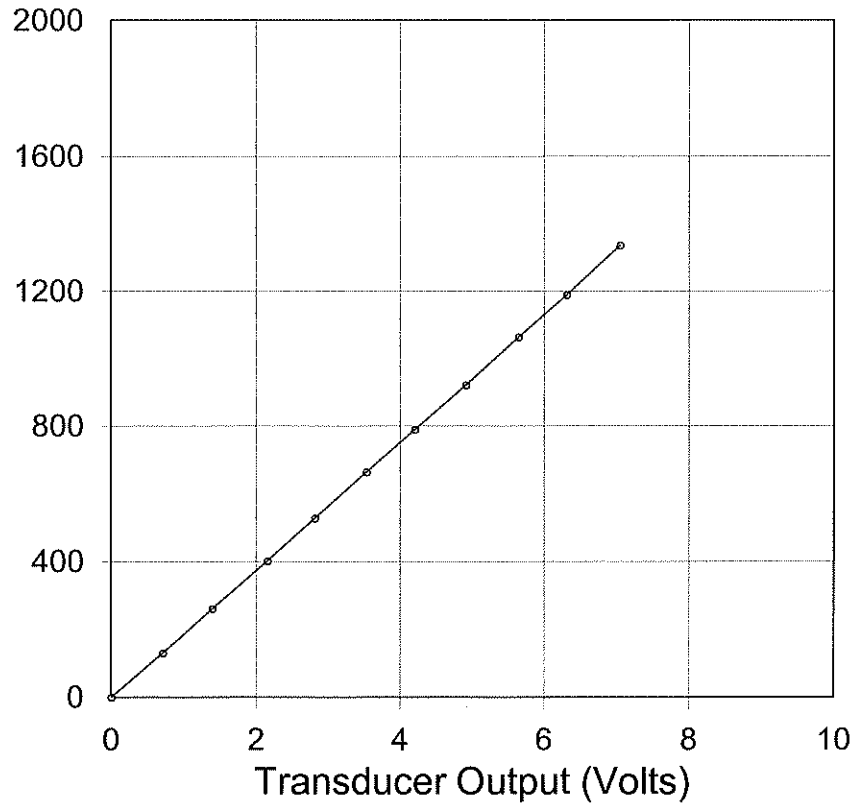

PDA Cal Factor (5.0 V)

94.5 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
132	0.70
261	1.39
402	2.15
527	2.81
664	3.53
789	4.20
921	4.91
1064	5.64
1189	6.30
1337	7.05

Shunt (60.4 K Ω)

2.5 V

General Factor

328.2 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Calibrated by: Kurt Huth

Calibrated on: 21-Dec-2009