




Pile Dynamics, Inc.

Pile Dynamics, Inc.

Transducer E798

Strain ($\mu\epsilon$)

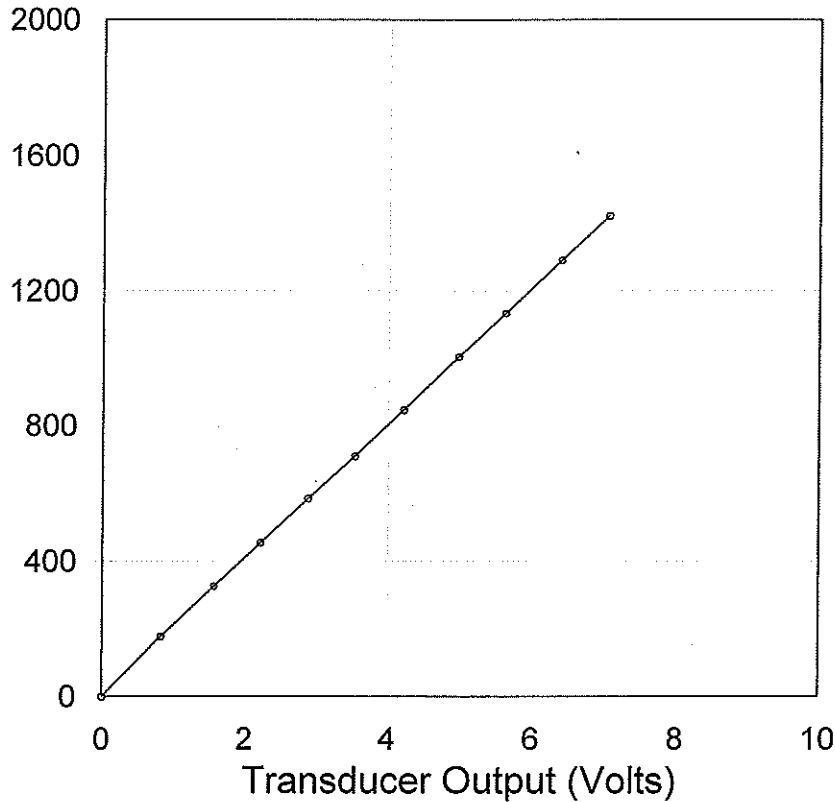

PDA Cal Factor (5.0 V)

100.2 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
179	0.82
326	1.56
454	2.21
583	2.87
708	3.53
846	4.21
1002	4.97
1134	5.62
1290	6.39
1423	7.05

Shunt (60.4 K Ω)

2.5 V

General Factor

347.9 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2011 Version 1.5

Calibrated by: *E.S. S...*

Calibrated on: 28-Nov-2012

Smart Sensor? Yes No Smart Chip

Programmed by: E.S. Date: 11-28-12 CRC value 61E3