




Pile Dynamics, Inc.

Transducer E799

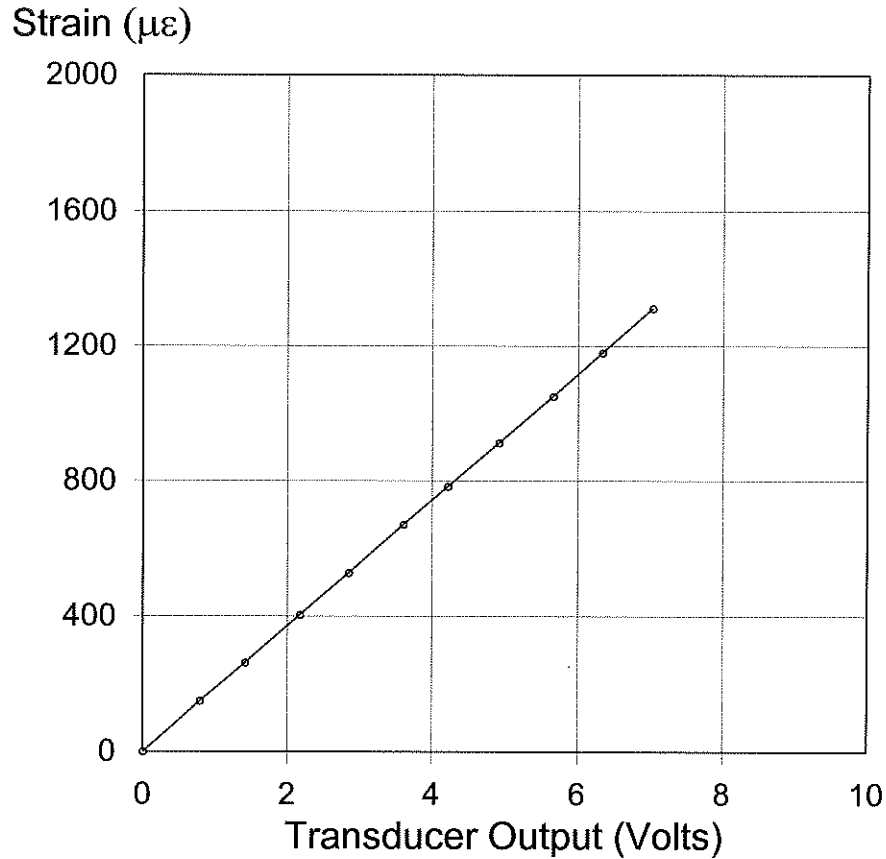

PDA Cal Factor (5.0 V) 93.2 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
150	0.78
262	1.41
403	2.17
527	2.85
670	3.60
783	4.21
911	4.91
1052	5.65
1181	6.33
1312	7.02

Shunt (60.4 K Ω) 2.5 V
 General Factor 323.5 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2009 Version 1.3

Calibrated by: *Atack*
 Calibrated on: 02-Mar-2010