




Pile Dynamics, Inc.

Pile Dynamics, Inc.

Transducer E983

Strain ($\mu\epsilon$)

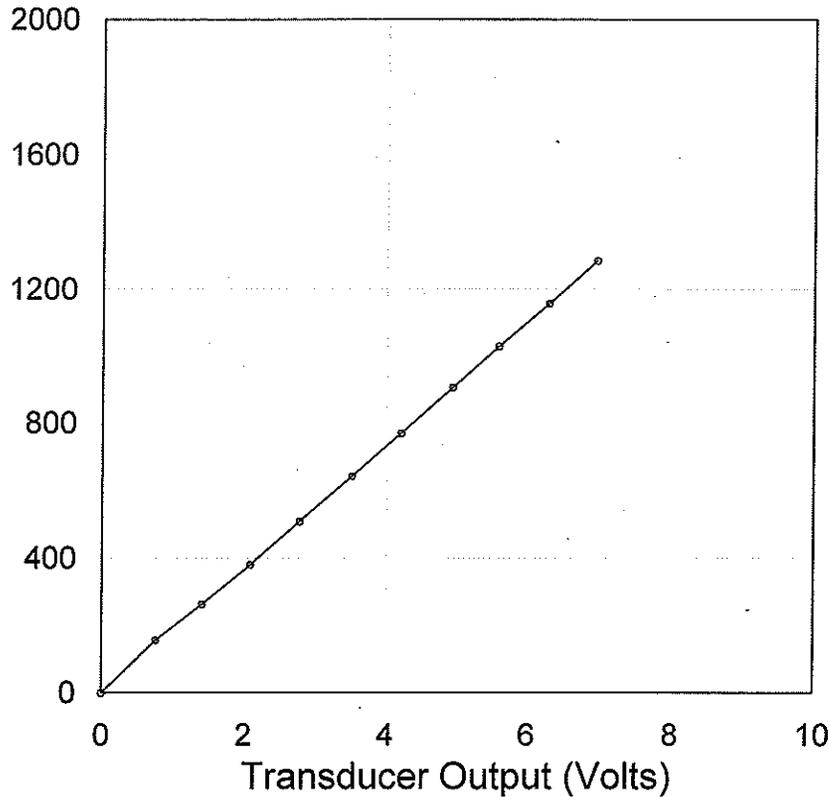

PDA Cal Factor (5.0 V)

91.8 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
157	0.76
263	1.41
380	2.08
507	2.77
642	3.50
770	4.20
906	4.93
1028	5.58
1157	6.27
1284	6.95

Shunt (60.4 K Ω)

2.5 V

General Factor

318.7 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2011 Version 1.5

Calibrated by:

Calibrated on:

22-Mar-2013

Smart Sensor? Yes No Smart Chip

Programmed by: E.S. Date: 3-22-13 CRC value 46A9