




Pile Dynamics, Inc.

Transducer E986

Strain ($\mu\epsilon$)

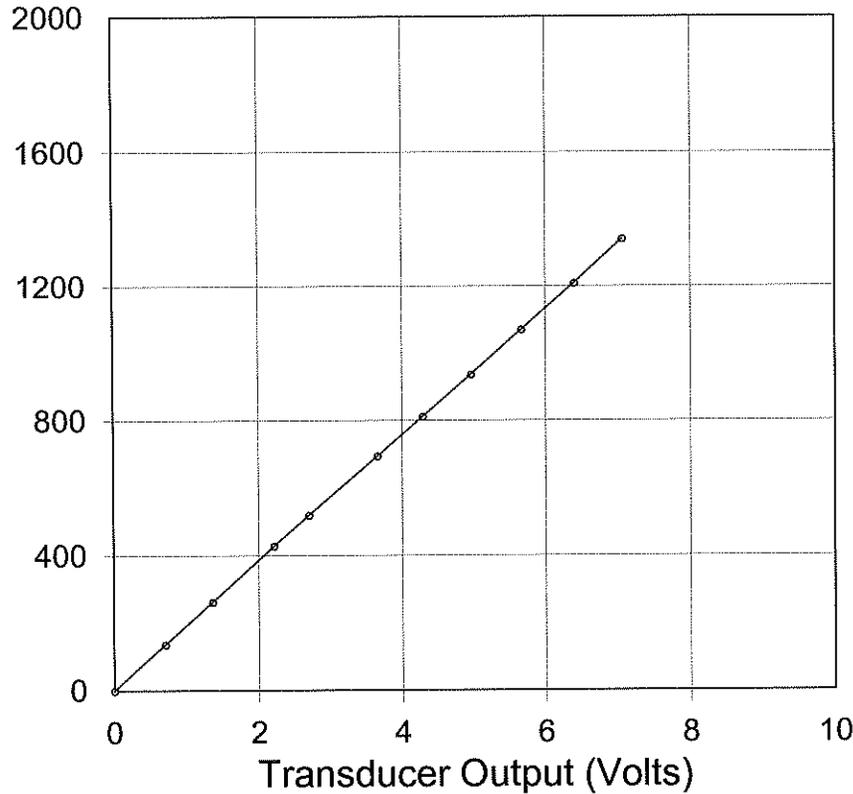

PDA Cal Factor (5.0 V)

94.3 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
138	0.70
262	1.36
428	2.22
518	2.70
693	3.65
810	4.28
937	4.96
1070	5.66
1208	6.39
1342	7.06

Shunt (60.4 K Ω)
General Factor

2.5 V
327.3 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2009 Version 1.3

Calibrated by:
Calibrated on:

02-Mar-2010