


Pile Dynamics, Inc.

Transducer E987

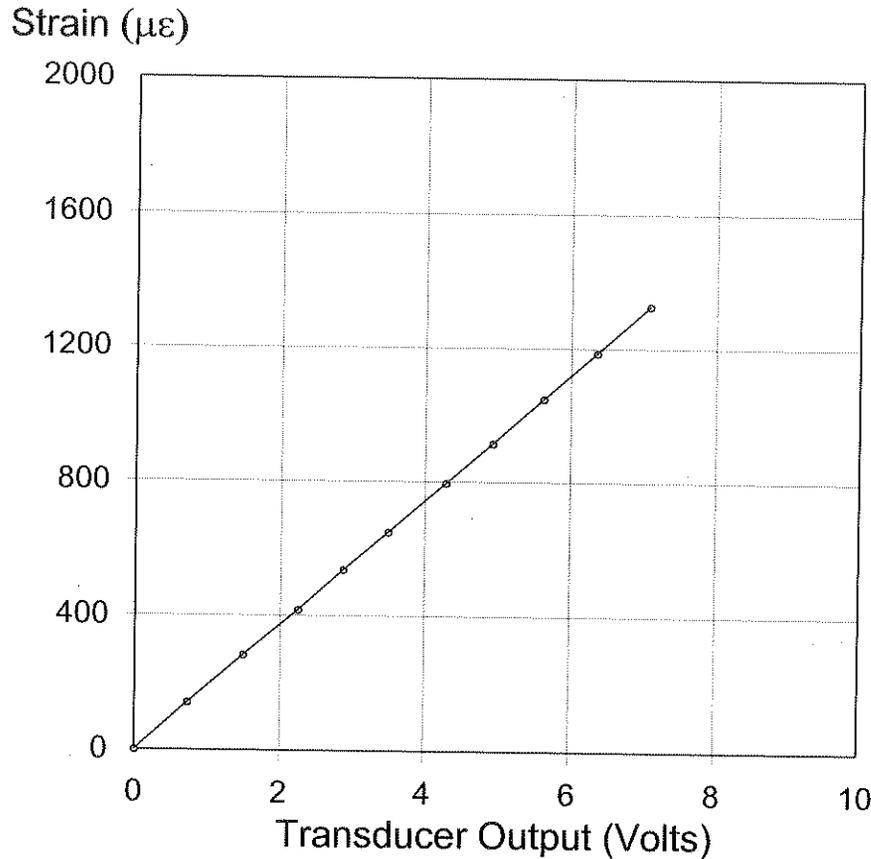

PDA Cal Factor (5.0 V) 93.2με/V

Applied Strain (με)	Transducer Output (Volts)
0	0.00
141	0.72
282	1.48
418	2.24
535	2.87
648	3.49
796	4.28
914	4.92
1048	5.62
1186	6.35
1327	7.08

Shunt (60.4 KΩ) 2.5 V
 General Factor 323.6με/mV/V

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2009 Version 1.3

Calibrated by: *Chack*
 Calibrated on: 05-Jan-2010

Smart Sensor? yes no Smart Chip programmed by: VT on: 1-5-10 CRC value: 693F