


Pile Dynamics, Inc.

Pile Dynamics, Inc.

Transducer

E996

Strain ($\mu\epsilon$)

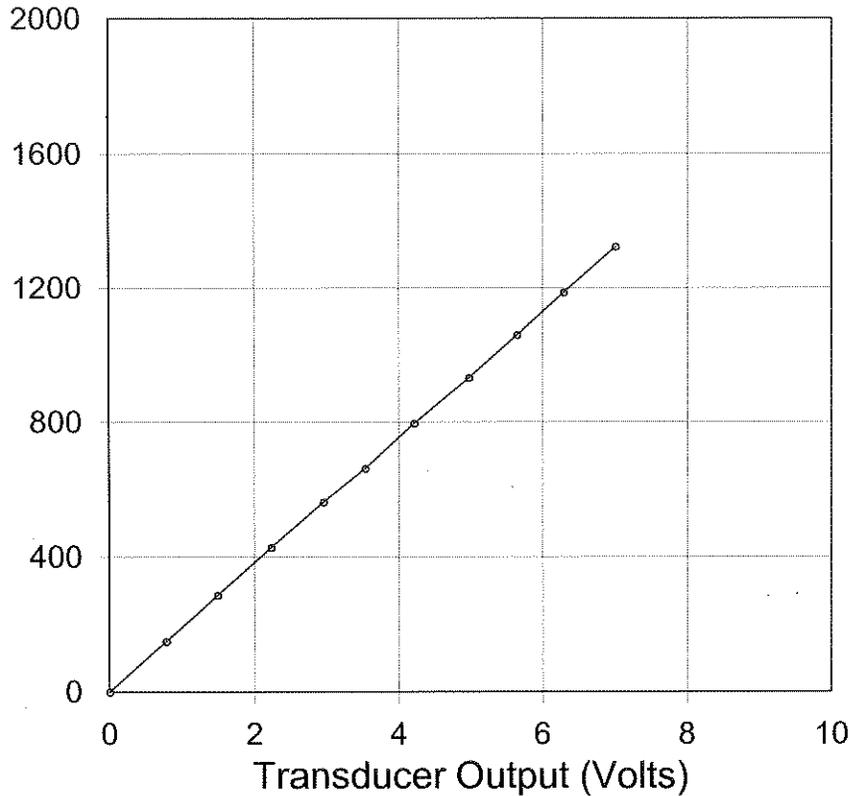

PDA Cal Factor (5.0 V)

93.9 $\mu\epsilon$ /V

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
149	0.78
287	1.49
427	2.23
561	2.96
662	3.53
795	4.21
931	4.97
1060	5.64
1188	6.29
1324	7.01

Shunt (60.4 K Ω)

2.5 V

General Factor

326.1 $\mu\epsilon$ /mV/V

Traceable to N.I.S.T.

Calibrated by: *[Signature]*

Calibrated on:

23-Feb-2010

Strain Transducer Calibrator System 2009 Version 1.3

Smart Sensor? yes no Smart Chip programmed by: VT on: 2-23-10 CRC value: 1093