

Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K15143 Temperature: 22.8 °C
 Model: KICHER PR Humidity: 27%
 Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

408.5 mv/5000g
 (81.7 μ v/g)
 R²: 0.999968 [Chip programmed]

Ref Acc 1: 85382! Cal on: 24Nov2025
 958 g's/volt
 Ref Acc 2: 85363! Cal on: 14Nov2025
 1000 g's/volt

Operator: William Johnson


William Johnson

 Signed

Calibration valid 2 years

From: FEB 26 2026

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

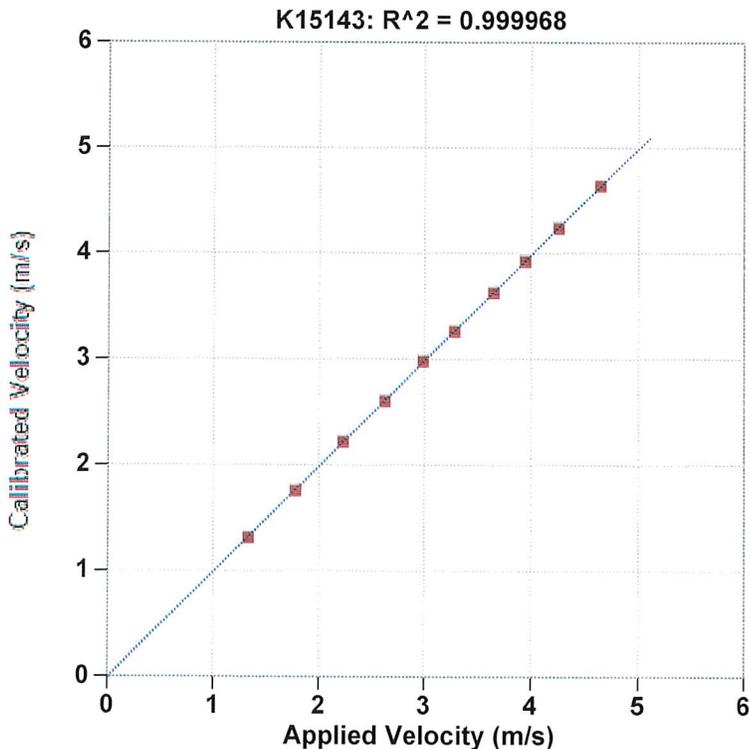

Reference Velocity	S/N K15143 Velocity
m/s	m/s
1.328	1.324
1.772	1.771
2.229	2.234
2.619	2.618
2.985	2.995
3.280	3.279
3.645	3.642
3.943	3.940
4.262	4.252
4.646	4.653

Maximum Acceleration: 1022 g's