

Certificate of Calibration Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K15145 **Temperature:** 22.8 °C
Model: KICHER PR **Humidity:** 27%
Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR
378.8 mv/5000g
 (75.8 μv/g)
 R²: 0.999947 [Chip programmed]

Ref Acc 1: 85382! **Cal on:** 24Nov2025
 958 g's/volt
Ref Acc 2: 85363! **Cal on:** 14Nov2025
 1000 g's/volt

Operator: William Johnson


William Johnson

 Signed

Calibration valid 2 years

From: FEB 26 2026

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

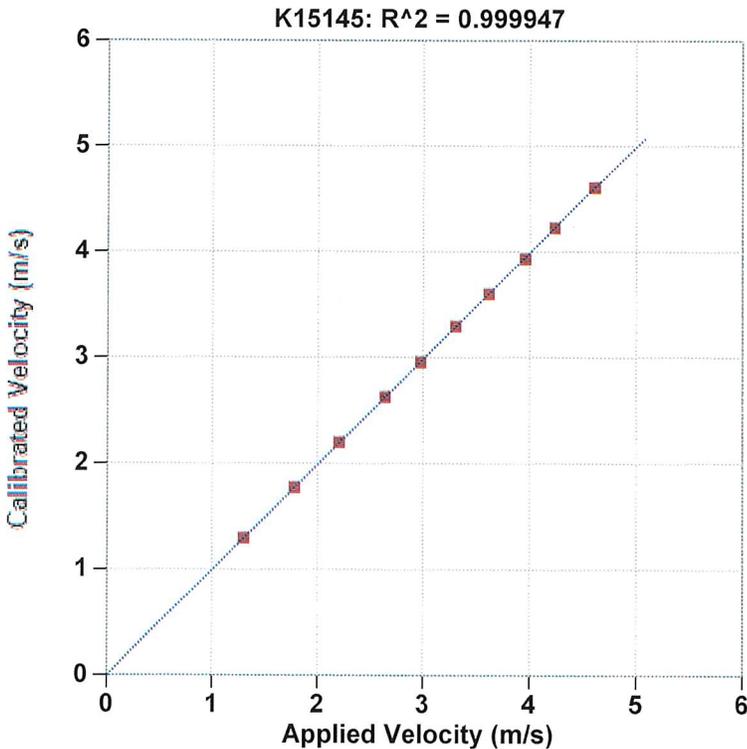

Reference Velocity m/s	S/N K15145 Velocity m/s
1.295	1.305
1.777	1.786
2.201	2.211
2.634	2.638
2.972	2.971
3.306	3.308
3.617	3.614
3.957	3.942
4.238	4.238
4.617	4.618

Maximum Acceleration: 1015 g's