


# Certificate of Calibration Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

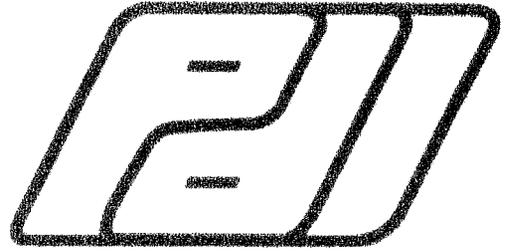

Serial No: LW383795      Temperature: 23.3 °C  
 Model: PIT ACC      Humidity: 39%  
 Calibrated on: Channel 4 on 8G 5161 LE

**PDA CALIBRATION FACTOR**  
 10.1 g's/volt  
 R<sup>2</sup>: 0.999914 [No chip]

Ref Acc 1: LW547722!      Cal on: 21Oct2025  
 10 g's/volt  
 Ref Acc 2: LW547723!      Cal on: 21Oct2025  
 10 g's/volt


Operator: William Johnson

Signed

Calibration valid 2 years

From: 19Feb2026

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

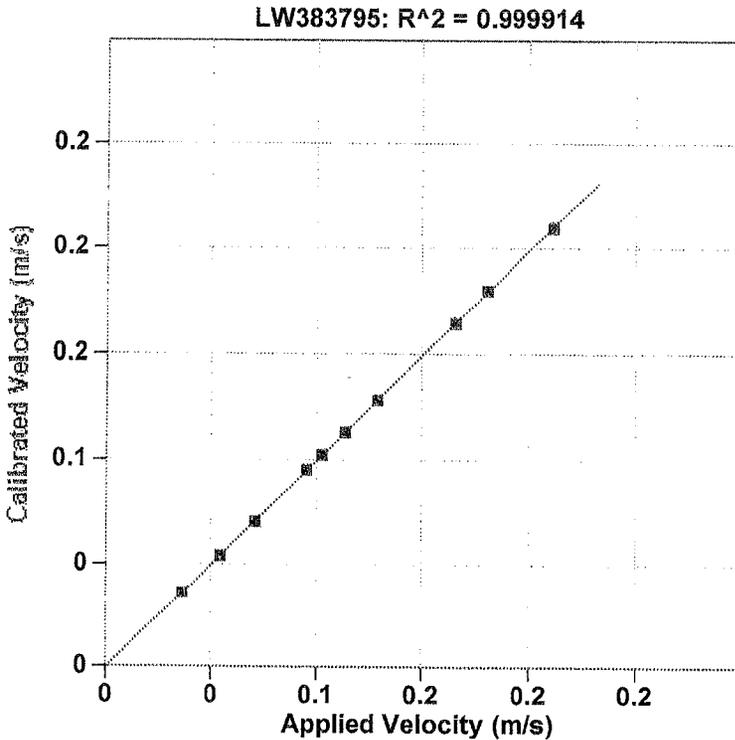

Reference Velocity	S/N LW383795 Velocity
m/s	m/s
0.036	0.037
0.054	0.055
0.071	0.071
0.095	0.096
0.102	0.103
0.113	0.113
0.129	0.129
0.166	0.165
0.180	0.181
0.211	0.210

Maximum Acceleration: 25 g's