




# Certificate of Calibration

Pile Dynamics, Inc.  
 Transducer Model: PDI Strain Transducer  
 Serial Number: 243C  
 PDI Gage Factor: 148.5  
 Mean Linear Correlation Coefficient: 0.999777

Table 1: Representative Calibration Data

Applied strain ( $\mu\text{E}$ )	Gage Output (mV/Vexc)	Applied strain ( $\mu\text{E}$ )	Gage Output (mV/Vexc)
-2106.3	-4.207	623.4	1.198
-1548.6	-3.085	931.8	1.795
-977.7	-1.967	1246.7	2.394
-479.0	-0.974	1574.8	3.000
-164.0	-0.355	1911.6	3.614
262.5	0.496	2021.0	3.802

Calibration Curve

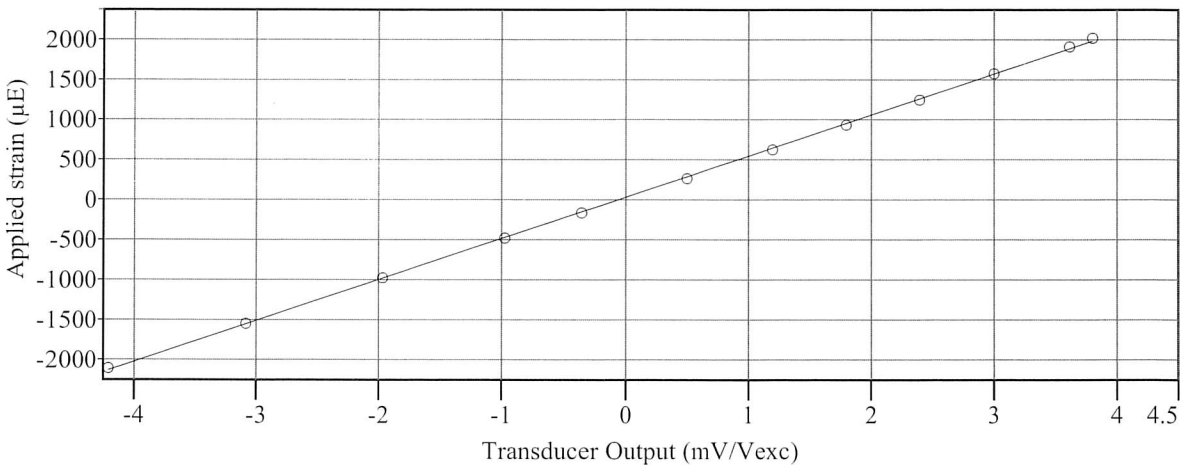

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Kelly Beal

Signature: \_\_\_\_\_

PDI Gage: 243C

Calibration Date:                     MAR 05 2026                    

