




Certificate of Calibration

Pile Dynamics, Inc.
 Transducer Model: PDI Strain Transducer
 Serial Number: 245C
 PDI Gage Factor: 147.4
 Mean Linear Correlation Coefficient: 0.999689

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-2158.8	-4.354	682.4	1.332
-1581.4	-3.178	1003.9	1.946
-997.4	-2.014	1340.8	2.569
-479.0	-0.967	1679.8	3.193
-137.8	-0.292	2014.4	3.804
282.2	0.538		

Calibration Curve

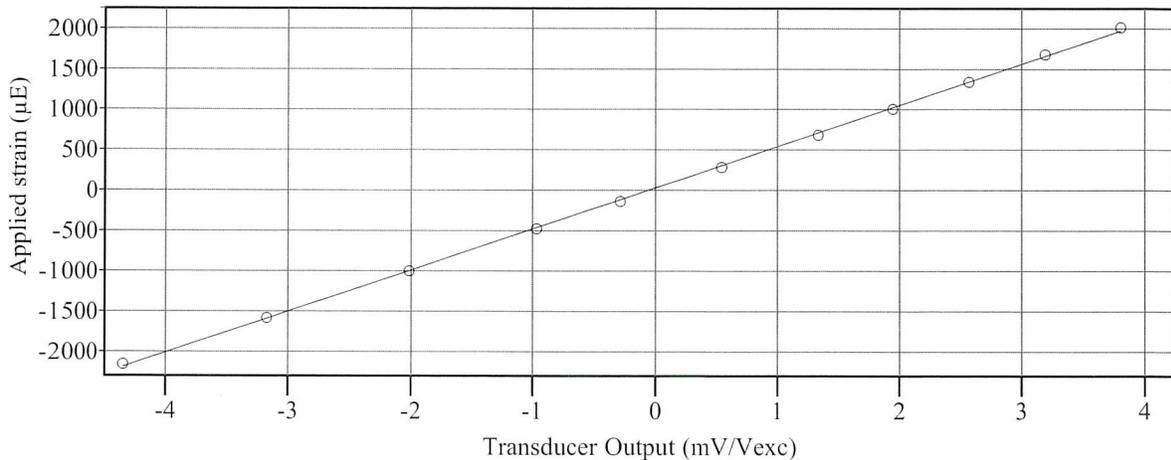

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Kelly Beal

Signature: 

PDI Gage: 245C

Calibration Date: FEB 27 2026

