




Certificate of Calibration

Pile Dynamics, Inc.
 Transducer Model: PDI Strain Transducer
 Serial Number: 325C
 PDI Gage Factor: 96.3
 Mean Linear Correlation Coefficient: 0.999956

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-2040.7	-6.168	706.5	2.122
-1568.2	-4.747	951.4	2.856
-1089.2	-3.301	1187.7	3.556
-614.6	-1.876	1443.6	4.303
-183.7	-0.579	1706.0	5.075
78.7	0.224	2014.4	5.963
400.3	1.212		

Calibration Curve

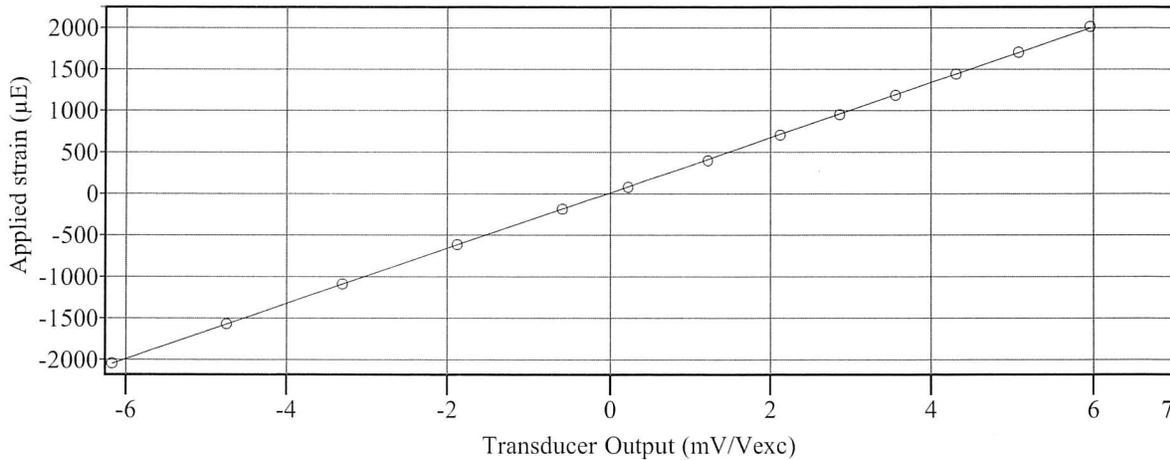

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Kelly Beal
 PDI Gage: 325C
 Calibration Date: _____

Signature: _____

MAR 25 2026

