


Certificate of Calibration Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

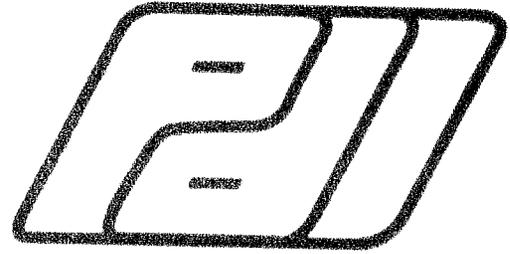

Serial No: 5567 Temperature: 22.5 °C
 Model: KICHER PR Humidity: 25%
 Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

335.8 mv/5000g
 (67.2 μ v/g)
 R²: 0.999944 [Chip programmed]

Ref Acc 1: 85382! Cal on: 24Nov2025
 958 g's/volt
 Ref Acc 2: 85363! Cal on: 14Nov2025
 1000 g's/volt


Operator: William Johnson

William Johnson
 Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 11Feb2026

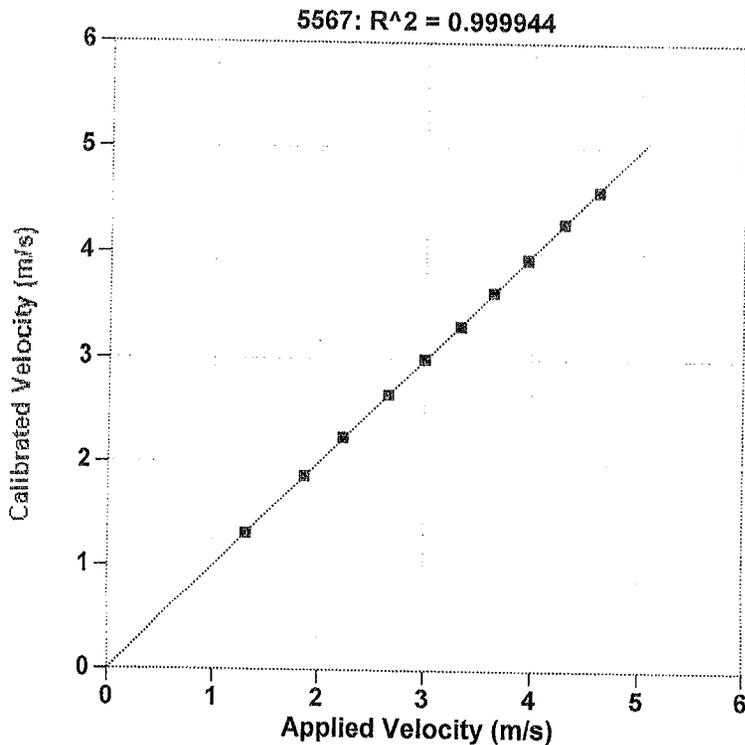

Reference Velocity	S/N 5567 Velocity
m/s	m/s
1.312	1.316
1.865	1.868
2.234	2.248
2.656	2.656
2.994	2.999
3.326	3.319
3.630	3.638
3.950	3.952
4.290	4.290
4.615	4.600

Maximum Acceleration: 1023 g's